

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location Alamance Co. Jail
Instrument Serial No. 008853 107 S Maple St
Greensboro NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 14th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. A. Bryant

Signature of Certifying Official

1671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008853 Test Record Number: 3303
Test Date: 02/18/2021 Test Time: 3:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:19pm
FLO	Pass	3:19pm
FC	Pass	3:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:19pm
SRC	Pass	3:19pm
DET	Pass	3:19pm
BAR	Pass	3:19pm
BT	Pass	3:19pm

Blank Tests

Test	Status	Time
AIR	Pass	3:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:20pm

CRC Tests

Test	Status	Time
COMP	Pass	3:20pm
CAL	Pass	3:20pm

Preventive Maintenance
Status: Pass

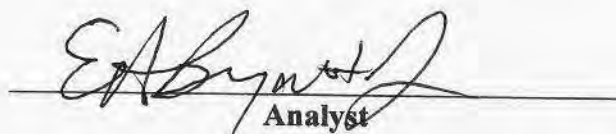
Analyst

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008853

Test Date: 02/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	3:07pm
AIR BLK	.00	3:08pm
ACCY CHK	.08	3:09pm
AIR BLK	.00	3:10pm
SUB TEST	.00	3:11pm
AIR BLK	.00	3:12pm
SUB TEST	.00	3:13pm
AIR BLK	.00	3:14pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Alamance Instrument Location Alamance Co Jail

Instrument Serial No. 008913 109 S. Maple St
GRATON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



EAB [Signature] Signature of Certifying Official 691 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913
Test Date: 02/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	3:09pm
AIR BLK	.00	3:10pm
ACCY CHK	.07	3:10pm
AIR BLK	.00	3:11pm
SUB TEST	.00	3:12pm
AIR BLK	.00	3:13pm
SUB TEST	.00	3:14pm
AIR BLK	.00	3:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913 Test Record Number: 4163
Test Date: 02/18/2021 Test Time: 3:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:19pm
FLO	Pass	3:19pm
FC	Pass	3:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:19pm
SRC	Pass	3:19pm
DET	Pass	3:19pm
BAR	Pass	3:19pm
BT	Pass	3:19pm

Blank Tests

Test	Status	Time
AIR	Pass	3:20pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:20pm

CRC Tests

Test	Status	Time
COMP	Pass	3:20pm
CAL	Pass	3:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Avery Instrument Location Banner EIK PD
Instrument Serial No. 008724 Banner EIK, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724
Test Date: 02/23/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG920301

Exp Date: 07/21/2021

Test	g/210L	Time
DIAG	Pass	3:32pm
AIR BLK	.00	3:33pm
ACCY CHK	.08	3:33pm
AIR BLK	.00	3:34pm
SUB TEST	.00	3:35pm
AIR BLK	.00	3:36pm
SUB TEST	.00	3:37pm
AIR BLK	.00	3:38pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

AVERY COUNTY BANNER ELK PD 050

Serial Number: 008724 Test Record Number: 655
Test Date: 02/23/2021 Test Time: 3:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:40pm
FLO	Pass	3:40pm
FC	Pass	3:40pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:41pm
SRC	Pass	3:41pm
DET	Pass	3:41pm
BAR	Pass	3:41pm
BT	Pass	3:41pm

Blank Tests

Test	Status	Time
AIR	Pass	3:41pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:41pm

CRC Tests

Test	Status	Time
COMP	Pass	3:41pm
CAL	Pass	3:41pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County BLADEN Instrument Location BLADEN COUNTY
Instrument Serial No. 008818 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 04 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008818
Test Date: 02/04/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	2:08pm
AIR BLK	.00	2:09pm
ACCY CHK	.08	2:10pm
AIR BLK	.00	2:11pm
SUB TEST	.00	2:12pm
AIR BLK	.00	2:13pm
SUB TEST	.00	2:14pm
AIR BLK	.00	2:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008818 Test Record Number: 1732
Test Date: 02/04/2021 Test Time: 2:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:16pm
FLO	Pass	2:16pm
FC	Pass	2:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:17pm
SRC	Pass	2:17pm
DET	Pass	2:17pm
BAR	Pass	2:17pm
BT	Pass	2:17pm

Blank Tests

Test	Status	Time
AIR	Pass	2:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:17pm

CRC Tests

Test	Status	Time
COMP	Pass	2:17pm
CAL	Pass	2:17pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County BLADEN Instrument Location BLADEN COUNTY
Instrument Serial No. 008894 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 04 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan Rg Bann
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008894
Test Date: 02/04/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	2:11pm
AIR BLK	.00	2:12pm
ACCY CHK	.08	2:13pm
AIR BLK	.00	2:15pm
SUB TEST	.00	2:15pm
AIR BLK	.00	2:16pm
SUB TEST	.00	2:17pm
AIR BLK	.00	2:18pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BLADEN COUNTY DETENTION CENTER 080

Serial Number: 008894 Test Record Number: 1279
Test Date: 02/04/2021 Test Time: 2:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:19pm
FLO	Pass	2:19pm
FC	Pass	2:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:19pm
SRC	Pass	2:19pm
DET	Pass	2:19pm
BAR	Pass	2:19pm
BT	Pass	2:19pm

Blank Tests

Test	Status	Time
AIR	Pass	2:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:20pm

CRC Tests

Test	Status	Time
COMP	Pass	2:20pm
CAL	Pass	2:20pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County BRUNSWICK Instrument Location LELAND
Instrument Serial No. 008787 POLICE DEPT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Barnes
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BRUNSWICK COUNTY LELAND PD 090

Serial Number: 008787
Test Date: 02/16/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	2:02pm
AIR BLK	.00	2:03pm
ACCY CHK	.07	2:04pm
AIR BLK	.00	2:04pm
SUB TEST	.00	2:05pm
AIR BLK	.00	2:06pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BRUNSWICK COUNTY LELAND PD 090

Serial Number: 008787 Test Record Number: 873
Test Date: 02/16/2021 Test Time: 2:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:09pm
FLO	Pass	2:09pm
FC	Pass	2:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:10pm
SRC	Pass	2:10pm
DET	Pass	2:10pm
BAR	Pass	2:10pm
BT	Pass	2:10pm

Blank Tests

Test	Status	Time
AIR	Pass	2:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:10pm

CRC Tests

Test	Status	Time
COMP	Pass	2:11pm
CAL	Pass	2:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Buncombe Instrument Location Black Mountain PD

Instrument Serial No. 008697 Black Mountain, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 17 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BUNCOMBE COUNTY BLACK MOUNTAIN PD 100

Serial Number: 008697
Test Date: 02/17/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933901
Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	2:23pm
AIR BLK	.00	2:24pm
ACCY CHK	.08	2:25pm
AIR BLK	.00	2:26pm
SUB TEST	.00	2:27pm
AIR BLK	.00	2:28pm
SUB TEST	.00	2:29pm
AIR BLK	.00	2:30pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

BUNCOMBE COUNTY BLACK MOUNTAIN PD 100

Serial Number: 008697 Test Record Number: 3946
Test Date: 02/17/2021 Test Time: 2:32pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:32pm
FLO	Pass	2:32pm
FC	Pass	2:33pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:33pm
SRC	Pass	2:33pm
DET	Pass	2:33pm
BAR	Pass	2:33pm
BT	Pass	2:33pm

Blank Tests

Test	Status	Time
AIR	Pass	2:33pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:33pm

CRC Tests

Test	Status	Time
COMP	Pass	2:34pm
CAL	Pass	2:34pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Burke Instrument Location Burke County Jail

Instrument Serial No. 008911 Morganton, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008911
Test Date: 02/10/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG920301

Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	9:38am
AIR BLK	.00	9:39am
ACCY CHK	.07	9:40am
AIR BLK	.00	9:41am
SUB TEST	.00	9:41am
AIR BLK	.00	9:42am
SUB TEST	.00	9:44am
AIR BLK	.00	9:45am

Reported AC: .00 g/210L

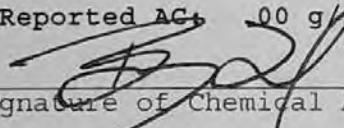
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

BURKE COUNTY BURKE COUNTY JAIL 110

Serial Number: 008911 Test Record Number: 651
Test Date: 02/10/2021 Test Time: 9:45am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:45am
FLO	Pass	9:45am
FC	Pass	9:46am

Temperature Tests

Test	Status	Time
FC1	Pass	9:46am
SRC	Pass	9:46am
DET	Pass	9:46am
BAR	Pass	9:46am
BT	Pass	9:46am

Blank Tests

Test	Status	Time
AIR	Pass	9:46am

Printer Tests

Test	Status	Time
PRNT	Pass	9:46am

CRC Tests

Test	Status	Time
COMP	Pass	9:47am
CAL	Pass	9:47am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Kannapolis PD
Instrument Serial No. 008589 401 Lurette Way, Kannapolis

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutchins
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY KANNAPOLIS PD 120

Serial Number: 008589

Test Date: 02/09/2021

Citation Number: M0000000-0

Subject's Name:

~~PREVENTIVE, MAINTENANCE~~

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test


Lot Number: AG007601

Exp Date: 03/16/2022

Test g/210L Time

DIAG	Pass	5:03pm
AIR BLK	.00	5:03pm
ACCY CHK	.08	5:04pm
AIR BLK	.00	5:05pm
SUB TEST	.00	5:05pm
AIR BLK	.00	5:06pm
SUB TEST	.00	5:08pm
AIR BLK	.00	5:09pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY KANNAPOLIS PD 120

Serial Number: 008589 Test Record Number: 3197
Test Date: 02/09/2021 Test Time: 5:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:10pm
FLO	Pass	5:10pm
FC	Pass	5:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:10pm
SRC	Pass	5:10pm
DET	Pass	5:10pm
BAR	Pass	5:10pm
BT	Pass	5:10pm

Blank Tests

Test	Status	Time
AIR	Pass	5:11pm

Printer Tests

Test	Status	Time
PRNT	Pass	5:11pm

CRC Tests

Test	Status	Time
COMP	Pass	5:11pm
CAL	Pass	5:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus County SO

Instrument Serial No. 008590 30 Corban Ave, Concord

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008590
Test Date: 02/23/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG920301

Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	2:13pm
AIR BLK	.00	2:14pm
ACCY CHK	.08	2:15pm
AIR BLK	.00	2:16pm
SUB TEST	.00	2:17pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:19pm
AIR BLK	.00	2:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008590 Test Record Number: 3696
Test Date: 02/23/2021 Test Time: 2:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:21pm
FLO	Pass	2:21pm
FC	Pass	2:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:22pm
SRC	Pass	2:22pm
DET	Pass	2:22pm
BAR	Pass	2:22pm
BT	Pass	2:22pm

Blank Tests

Test	Status	Time
AIR	Pass	2:22pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:22pm

CRC Tests

Test	Status	Time
COMP	Pass	2:22pm
CAL	Pass	2:22pm

Preventive Maintenance
Status: *Pass*


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cabarrus Instrument Location Cabarrus Co. 50

Instrument Serial No. 008792 30 Corban Ave, Concord

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Holt
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008792

Test Date: 02/05/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001


Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	3:46pm
AIR BLK	.00	3:47pm
ACCY CHK	.08	3:48pm
AIR BLK	.00	3:49pm
SUB TEST	.00	3:50pm
AIR BLK	.00	3:51pm
SUB TEST	.00	3:52pm
AIR BLK	.00	3:53pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

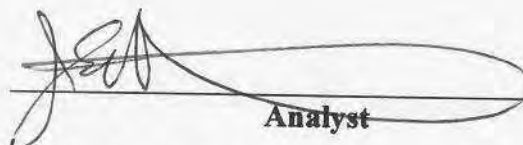
Analyst

Intox EC/IR-II: Preventive Maintenance

CABARRUS COUNTY CABARRUS COUNTY SO 120

Serial Number: 008792 Test Record Number: 3165
Test Date: 02/05/2021 Test Time: 3:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:55pm
FLO	Pass	3:55pm
FC	Pass	3:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:55pm
SRC	Pass	3:55pm
DET	Pass	3:55pm
BAR	Pass	3:55pm
BT	Pass	3:55pm

Blank Tests

Test	Status	Time
AIR	Pass	3:55pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:55pm

CRC Tests

Test	Status	Time
COMP	Pass	3:56pm
CAL	Pass	3:56pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location Caldwell Co. Jail

Instrument Serial No. 008719 Lenoir, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008719
Test Date: 02/24/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	9:32am
AIR BLK	.00	9:33am
ACCY CHK	.07	9:34am
AIR BLK	.00	9:35am
SUB TEST	.00	9:35am
AIR BLK	.00	9:36am
SUB TEST	.00	9:38am
AIR BLK	.00	9:39am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008719 Test Record Number: 2761
Test Date: 02/24/2021 Test Time: 9:41am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:41am
FLO	Pass	9:41am
FC	Pass	9:41am

Temperature Tests

Test	Status	Time
FC1	Pass	9:41am
SRC	Pass	9:41am
DET	Pass	9:41am
BAR	Pass	9:41am
BT	Pass	9:41am

Blank Tests

Test	Status	Time
AIR	Pass	9:42am


Printer Tests

Test	Status	Time
PRNT	Pass	9:42am

CRC Tests

Test	Status	Time
COMP	Pass	9:42am
CAL	Pass	9:42am

Preventive Maintenance
Status: Pass

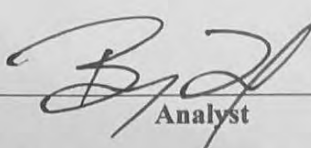

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location Caldwell Co Jail

Instrument Serial No. 008803 Lenoir, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008803
Test Date: 02/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022


Test	g/210L	Time
DIAG	Pass	9:13am
AIR BLK	.00	9:14am
ACCY CHK	.07	9:15am
AIR BLK	.00	9:16am
SUB TEST	.00	9:17am
AIR BLK	.00	9:18am
SUB TEST	.00	9:19am
AIR BLK	.00	9:20am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

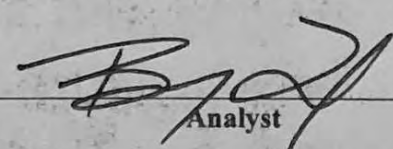

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008803 Test Record Number: 713
Test Date: 02/02/2021 Test Time: 9:21am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:22am
FLO	Pass	9:22am
FC	Pass	9:22am

Temperature Tests

Test	Status	Time
FC1	Pass	9:22am
SRC	Pass	9:22am
DET	Pass	9:22am
BAR	Pass	9:22am
BT	Pass	9:22am

Blank Tests

Test	Status	Time
AIR	Pass	9:23am


Printer Tests

Test	Status	Time
PRNT	Pass	9:23am

CRC Tests

Test	Status	Time
COMP	Pass	9:23am
CAL	Pass	9:23am

Preventive Maintenance
Status: Pass

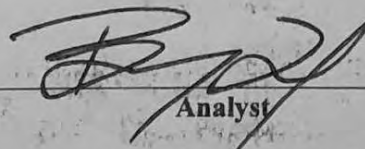

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Caldwell Instrument Location Caldwell Co. Jail

Instrument Serial No. 003916 Lenoir, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CALDWELL COUNTY CALDWELL COUNTY JAIL
130

Serial Number: 008916
Test Date: 02/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	9:40am
AIR BLK	.00	9:41am
ACCY CHK	.08	9:42am
AIR BLK	.00	9:44am
SUB TEST	.00	9:45am
AIR BLK	.00	9:46am
SUB TEST	.00	9:47am
AIR BLK	.00	9:48am

Reported AC: .00 g/210L

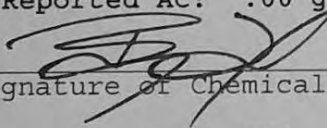

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CALDWELL COUNTY CALDWELL COUNTY JAIL 130

Serial Number: 008916 Test Record Number: 1552
Test Date: 02/02/2021 Test Time: 9:49am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:49am
FLO	Pass	9:49am
FC	Pass	9:49am

Temperature Tests

Test	Status	Time
FC1	Pass	9:49am
SRC	Pass	9:49am
DET	Pass	9:49am
BAR	Pass	9:49am
BT	Pass	9:49am

Blank Tests

Test	Status	Time
AIR	Pass	9:50am


Printer Tests

Test	Status	Time
PRNT	Pass	9:50am

CRC Tests

Test	Status	Time
COMP	Pass	9:50am
CAL	Pass	9:50am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Carteret Instrument Location Emerald Isle
Instrument Serial No. 008917 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008917
Test Date: 02/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	5:09pm
AIR BLK	.00	5:09pm
ACCY CHK	.07	5:10pm
AIR BLK	.00	5:11pm
SUB TEST	.00	5:12pm
AIR BLK	.00	5:13pm
SUB TEST	.00	5:14pm
AIR BLK	.00	5:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

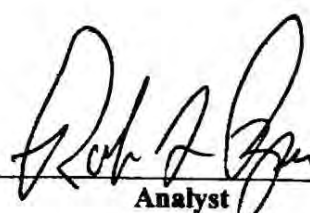

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CARTERET COUNTY EMERALD ISLE PD 150

Serial Number: 008917 Test Record Number: 905
Test Date: 02/18/2021 Test Time: 5:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:16pm
FLO	Pass	5:16pm
FC	Pass	5:16pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:16pm
SRC	Pass	5:16pm
DET	Pass	5:16pm
BAR	Pass	5:16pm
BT	Pass	5:16pm

Blank Tests

Test	Status	Time
AIR	Pass	5:17pm

Printer Tests


Test	Status	Time
PRNT	Pass	5:17pm

CRC Tests

Test	Status	Time
COMP	Pass	5:17pm
CAL	Pass	5:17pm

Preventive Maintenance

Status: Pass

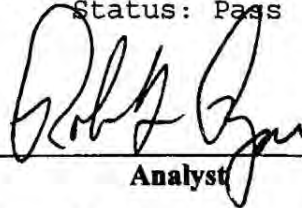

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Catawba Instrument Location Catawba County SO

Instrument Serial No. 008821 100 B Southwest Blvd, Newton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2020 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hatcher
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821

Test Date: 02/05/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	6:13pm
AIR BLK	.00	6:14pm
ACCY CHK	.07	6:14pm
AIR BLK	.00	6:15pm
SUB TEST	.00	6:16pm
AIR BLK	.00	6:17pm
SUB TEST	.00	6:18pm
AIR BLK	.00	6:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CATAWBA COUNTY CATAWBA COUNTY SO 170

Serial Number: 008821 Test Record Number: 2137
Test Date: 02/05/2021 Test Time: 6:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:21pm
FLO	Pass	6:21pm
FC	Pass	6:21pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:21pm
SRC	Pass	6:21pm
DET	Pass	6:21pm
BAR	Pass	6:21pm
BT	Pass	6:21pm

Blank Tests

Test	Status	Time
AIR	Pass	6:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:22pm

CRC Tests

Test	Status	Time
COMP	Pass	6:22pm
CAL	Pass	6:22pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Chowan Instrument Location Chowan Co Public Safety Center
Instrument Serial No. 008895 305 Freemason St, Eden, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 643 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895

Test Date: 02/04/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021


Test	g/210L	Time
DIAG	Pass	11:12am
AIR BLK	.00	11:13am
ACCY CHK	.07	11:13am
AIR BLK	.00	11:14am
SUB TEST	.00	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:17am
AIR BLK	.00	11:18am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895 Test Record Number: 1019
Test Date: 02/04/2021 Test Time: 11:20am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:21am
FLO	Pass	11:21am
FC	Pass	11:21am

Temperature Tests

Test	Status	Time
FC1	Pass	11:21am
SRC	Pass	11:21am
DET	Pass	11:21am
BAR	Pass	11:21am
BT	Pass	11:21am

Blank Tests

Test	Status	Time
AIR	Pass	11:21am

Printer Tests

Test	Status	Time
PRNT	Pass	11:21am

CRC Tests

Test	Status	Time
COMP	Pass	11:22am
CAL	Pass	11:22am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Clay Instrument Location Clay County Jail
Instrument Serial No. 008608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuthbert
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608
Test Date: 02/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:11am
AIR BLK	.00	11:12am
ACCY CHK	.08	11:13am
AIR BLK	.00	11:14am
SUB TEST	.00	11:15am
AIR BLK	.00	11:16am
SUB TEST	.00	11:19am
AIR BLK	.00	11:20am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608 Test Record Number: 1332
Test Date: 02/10/2021 Test Time: 11:23am EST

System Check: Passed

Baseline Tests

Test	Status	Time
IR	Pass	11:23am
FLO	Pass	11:23am
FC	Pass	11:23am

Temperature Tests

Test	Status	Time
FC1	Pass	11:23am
SRC	Pass	11:23am
DET	Pass	11:23am
BAR	Pass	11:23am
BT	Pass	11:23am

Blank Tests

Test	Status	Time
AIR	Pass	11:24am

Printer Tests

Test	Status	Time
PRNT	Pass	11:24am

CRC Tests

Test	Status	Time
COMP	Pass	11:24am
CAL	Pass	11:24am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Cleveland Instrument Location Cleveland 50-Annex
Instrument Serial No. 008694 407 McBrayer St, Shelby

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008694
Test Date: 02/05/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933901


Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	8:11pm
AIR BLK	.00	8:12pm
ACCY CHK	.08	8:12pm
AIR BLK	.00	8:13pm
SUB TEST	.00	8:14pm
AIR BLK	.00	8:15pm
SUB TEST	.00	8:16pm
AIR BLK	.00	8:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008694 Test Record Number: 1511
Test Date: 02/05/2021 Test Time: 8:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	8:18pm
FLO	Pass	8:18pm
FC	Pass	8:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	8:18pm
SRC	Pass	8:18pm
DET	Pass	8:18pm
BAR	Pass	8:18pm
BT	Pass	8:18pm

Blank Tests

Test	Status	Time
AIR	Pass	8:19pm


Printer Tests

Test	Status	Time
PRNT	Pass	8:19pm

CRC Tests

Test	Status	Time
COMP	Pass	8:19pm
CAL	Pass	8:19pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Cleveland Instrument Location Cleveland 50-Annex

Instrument Serial No. 008927 407 McBrayer St, Shelby

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hutch
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND SO-ANNEX
220

Serial Number: 008927
Test Date: 02/11/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933901

Exp Date: 12/05/2021


Test	g/210L	Time
DIAG	Pass	6:12pm
AIR BLK	.00	6:13pm
ACCY CHK	.08	6:14pm
AIR BLK	.00	6:15pm
SUB TEST	.00	6:16pm
AIR BLK	.00	6:17pm
SUB TEST	.00	6:18pm
AIR BLK	.00	6:19pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

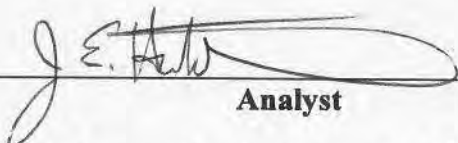

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CLEVELAND COUNTY CLEVELAND SO-ANNEX 220

Serial Number: 008927 Test Record Number: 653
Test Date: 02/11/2021 Test Time: 6:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:20pm
FLO	Pass	6:20pm
FC	Pass	6:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:21pm
SRC	Pass	6:21pm
DET	Pass	6:21pm
BAR	Pass	6:21pm
BT	Pass	6:21pm

Blank Tests

Test	Status	Time
AIR	Pass	6:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	6:21pm

CRC Tests

Test	Status	Time
COMP	Pass	6:21pm
CAL	Pass	6:21pm

Preventive Maintenance
Status: Pass

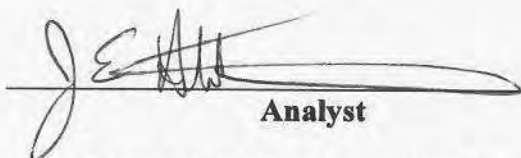

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County COLUMBUS Instrument Location TABOR CITY
Instrument Serial No. 008886 POLICE DEPT.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

COLUMBUS COUNTY TABOR CITY PD 230

Serial Number: 008886
Test Date: 02/24/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	2:14pm
AIR BLK	.00	2:15pm
ACCY CHK	.08	2:16pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:17pm
AIR BLK	.00	2:18pm
SUB TEST	.00	2:20pm
AIR BLK	.00	2:21pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

COLUMBUS COUNTY TABOR CITY PD 230

Serial Number: 008886 Test Record Number: 1573
Test Date: 02/24/2021 Test Time: 2:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:21pm
FLO	Pass	2:21pm
FC	Pass	2:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:22pm
SRC	Pass	2:22pm
DET	Pass	2:22pm
BAR	Pass	2:22pm
BT	Pass	2:22pm

Blank Tests

Test	Status	Time
AIR	Pass	2:22pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:22pm

CRC Tests

Test	Status	Time
COMP	Pass	2:23pm
CAL	Pass	2:23pm

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CUMBERLAND Instrument Location CUMBERLAND COUNTY
Instrument Serial No. 008614 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of FEBRUARY, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Basso
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008614
Test Date: 02/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:50am
AIR BLK	.00	10:51am
ACCY CHK	.07	10:52am
AIR BLK	.00	10:53am
SUB TEST	.00	10:54am
AIR BLK	.00	10:54am
SUB TEST	.00	10:56am
AIR BLK	.00	10:57am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008614 Test Record Number: 4479
Test Date: 02/02/2021 Test Time: 10:58am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:58am
FLO	Pass	10:58am
FC	Pass	10:58am

Temperature Tests

Test	Status	Time
FC1	Pass	10:58am
SRC	Pass	10:58am
DET	Pass	10:58am
BAR	Pass	10:58am
BT	Pass	10:58am

Blank Tests

Test	Status	Time
AIR	Pass	10:59am


Printer Tests

Test	Status	Time
PRNT	Pass	10:59am

CRC Tests

Test	Status	Time
COMP	Pass	10:59am
CAL	Pass	10:59am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CUMBERLAND Instrument Location CUMBERLAND COUNTY
Instrument Serial No. 008632 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alex R. Barnes

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008632

Test Date: 02/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Alvin R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:53am
AIR BLK	.00	10:54am
ACCY CHK	.08	10:54am
AIR BLK	.00	10:56am
SUB TEST	.00	10:57am
AIR BLK	.00	10:57am
SUB TEST	.00	10:59am
AIR BLK	.00	11:00am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008632 Test Record Number: 4331
Test Date: 02/02/2021 Test Time: 11:01am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:01am
FLO	Pass	11:01am
FC	Pass	11:02am

Temperature Tests

Test	Status	Time
FC1	Pass	11:02am
SRC	Pass	11:02am
DET	Pass	11:02am
BAR	Pass	11:02am
BT	Pass	11:02am

Blank Tests

Test	Status	Time
AIR	Pass	11:02am


Printer Tests

Test	Status	Time
PRNT	Pass	11:02am

CRC Tests

Test	Status	Time
COMP	Pass	11:02am
CAL	Pass	11:02am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County CUMBERLAND Instrument Location CUMBERLAND COUNTY
Instrument Serial No. 008633 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Burns

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008633
Test Date: 02/02/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:47am
AIR BLK	.00	10:48am
ACCY CHK	.07	10:48am
AIR BLK	.00	10:49am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:53am
AIR BLK	.00	10:54am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008633 Test Record Number: 5680
Test Date: 02/02/2021 Test Time: 10:54am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:55am
FLO	Pass	10:55am
FC	Pass	10:55am

Temperature Tests

Test	Status	Time
FC1	Pass	10:55am
SRC	Pass	10:55am
DET	Pass	10:55am
BAR	Pass	10:55am
BT	Pass	10:55am

Blank Tests

Test	Status	Time
AIR	Pass	10:55am

Printer Tests

Test	Status	Time
PRNT	Pass	10:55am

CRC Tests

Test	Status	Time
COMP	Pass	10:56am
CAL	Pass	10:56am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County CUMBERLAND Instrument Location CUMBERLAND COUNTY
Instrument Serial No. 008672 DETENTION CENTER

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 02 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. Burns

Signature of Certifying Official

648

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008672
Test Date: 02/02/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Alvin R
Permit Number: 0014-6279
Effective:
10/09/2020-10/09/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:48am
AIR BLK	.00	10:49am
ACCY CHK	.07	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:53am
AIR BLK	.00	10:54am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CUMBERLAND COUNTY DETENTION CENTER 250

Serial Number: 008672 Test Record Number: 7192
Test Date: 02/02/2021 Test Time: 10:57am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:57am
FLO	Pass	10:57am
FC	Pass	10:57am

Temperature Tests

Test	Status	Time
FC1	Pass	10:57am
SRC	Pass	10:57am
DET	Pass	10:57am
BAR	Pass	10:57am
BT	Pass	10:57am

Blank Tests

Test	Status	Time
AIR	Pass	10:58am

Printer Tests

Test	Status	Time
PRNT	Pass	10:58am

CRC Tests

Test	Status	Time
COMP	Pass	10:58am
CAL	Pass	10:58am

Preventive Maintenance
Status: Pass



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County DAVIE Instrument Location DAVIE CO. JAIL

Instrument Serial No. 008905 MOCKSVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008905
Test Date: 02/05/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	3:14pm
AIR BLK	.00	3:15pm
ACCY CHK	.08	3:15pm
AIR BLK	.00	3:16pm
SUB TEST	.00	3:17pm
AIR BLK	.00	3:18pm
SUB TEST	.00	3:20pm
AIR BLK	.00	3:20pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

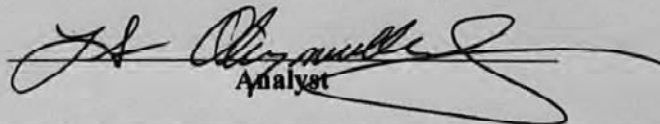
Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

DAVIE COUNTY DAVIE COUNTY JAIL 290

Serial Number: 008905 Test Record Number: 2533
Test Date: 02/05/2021 Test Time: 3:21pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:22pm
FLO	Pass	3:22pm
FC	Pass	3:22pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:22pm
SRC	Pass	3:22pm
DET	Pass	3:22pm
BAR	Pass	3:22pm
BT	Pass	3:22pm

Blank Tests

Test	Status	Time
AIR	Pass	3:23pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:23pm

CRC Tests

Test	Status	Time
COMP	Pass	3:23pm
CAL	Pass	3:23pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Franklin Instrument Location Franklin Co. LEC

Instrument Serial No. 008933 285 T. Kemp Rd
Louisburg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Ed Boyath

Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008933
Test Date: 02/16/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022

Test	g/210L	Time
DIAG	Pass	4:45pm
AIR BLK	.00	4:46pm
ACCY CHK	.07	4:46pm
AIR BLK	.00	4:47pm
SUB TEST	.00	4:48pm
AIR BLK	.00	4:49pm
SUB TEST	.00	4:51pm
AIR BLK	.00	4:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008933 Test Record Number: 1252
Test Date: 02/16/2021 Test Time: 4:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:53pm
FLO	Pass	4:53pm
FC	Pass	4:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:53pm
SRC	Pass	4:53pm
DET	Pass	4:53pm
BAR	Pass	4:53pm
BT	Pass	4:53pm

Blank Tests

Test	Status	Time
AIR	Pass	4:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:54pm

CRC Tests

Test	Status	Time
COMP	Pass	4:54pm
CAL	Pass	4:54pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Franklin Instrument Location Franklin Co LEC

Instrument Serial No. 008942 285 T-Komp Rd

Louisburg, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E. B. Boyd
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008942

Test Date: 02/16/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018202

Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	4:43pm
AIR BLK	.00	4:44pm
ACCY CHK	.07	4:44pm
AIR BLK	.00	4:45pm
SUB TEST	.00	4:46pm
AIR BLK	.00	4:47pm
SUB TEST	.00	4:49pm
AIR BLK	.00	4:50pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

FRANKLIN COUNTY FRANKLIN CO. LEC 340

Serial Number: 008942 Test Record Number: 2202
Test Date: 02/16/2021 Test Time: 4:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:51pm
FLO	Pass	4:51pm
FC	Pass	4:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:51pm
SRC	Pass	4:51pm
DET	Pass	4:51pm
BAR	Pass	4:51pm
BT	Pass	4:51pm

Blank Tests

Test	Status	Time
AIR	Pass	4:51pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:51pm

CRC Tests

Test	Status	Time
COMP	Pass	4:52pm
CAL	Pass	4:52pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Gates Instrument Location Gates C.S.O.

Instrument Serial No. 008884 202 Court St, Gatesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1st day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GATES COUNTY GATES CO SO 360

Serial Number: 008884
Test Date: 02/01/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:59am
AIR BLK	.00	12:00pm
ACCY CHK	.07	12:01pm
AIR BLK	.00	12:02pm
SUB TEST	.00	12:03pm
AIR BLK	.00	12:04pm
SUB TEST	.00	12:05pm
AIR BLK	.00	12:06pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

GATES COUNTY GATES CO SO 360

Serial Number: 008884 Test Record Number: 989
Test Date: 02/01/2021 Test Time: 12:08pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:09pm
FLO	Pass	12:09pm
FC	Pass	12:09pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:09pm
SRC	Pass	12:09pm
DET	Pass	12:09pm
BAR	Pass	12:09pm
BT	Pass	12:09pm

Blank Tests

Test	Status	Time
AIR	Pass	12:09pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:09pm

CRC Tests

Test	Status	Time
COMP	Pass	12:10pm
CAL	Pass	12:10pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location HIGH POINT TAIL

Instrument Serial No. 008655 HIGH POINT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1069
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY HIGH POINT JAIL 400

Serial Number: 008655
Test Date: 02/11/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	9:17am
AIR BLK	.00	9:18am
ACCY CHK	.08	9:19am
AIR BLK	.00	9:20am
SUB TEST	.00	9:21am
AIR BLK	.00	9:22am
SUB TEST	.00	9:23am
AIR BLK	.00	9:24am

Reported AC: .00 g/210L

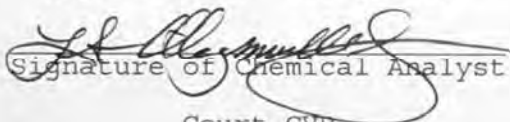
Signature of Chemical Analyst
Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY HIGH POINT JAIL 400

Serial Number: 008655 Test Record Number: 3649
Test Date: 02/11/2021 Test Time: 9:25am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:26am
FLO	Pass	9:26am
FC	Pass	9:26am

Temperature Tests

Test	Status	Time
FC1	Pass	9:26am
SRC	Pass	9:26am
DET	Pass	9:26am
BAR	Pass	9:26am
BT	Pass	9:26am

Blank Tests

Test	Status	Time
AIR	Pass	9:26am

Printer Tests

Test	Status	Time
PRNT	Pass	9:26am

CRC Tests

Test	Status	Time
COMP	Pass	9:27am
CAL	Pass	9:27am

Preventive Maintenance
Status: Pass

Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County GUILFORD Instrument Location HIGH POINT
Instrument Serial No. 00882B POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY HIGH POINT PD 401

Serial Number: 008828
Test Date: 02/11/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018401
Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	9:56am
AIR BLK	.00	9:57am
ACCY CHK	.08	9:57am
AIR BLK	.00	9:59am
SUB TEST	.00	9:59am
AIR BLK	.00	10:00am
SUB TEST	.00	10:02am
AIR BLK	.00	10:02am

Reported AC: .00 g/210L


Signature of Chemical Analyst
Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY HIGH POINT PD 401

Serial Number: 008828 Test Record Number: 3600
Test Date: 02/11/2021 Test Time: 10:04am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:04am
FLO	Pass	10:04am
FC	Pass	10:04am

Temperature Tests

Test	Status	Time
FC1	Pass	10:04am
SRC	Pass	10:04am
DET	Pass	10:04am
BAR	Pass	10:04am
BT	Pass	10:04am

Blank Tests

Test	Status	Time
AIR	Pass	10:05am


Printer Tests

Test	Status	Time
PRNT	Pass	10:05am

CRC Tests

Test	Status	Time
COMP	Pass	10:05am
CAL	Pass	10:05am

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County GUILFORD Instrument Location GREENSBORO JAIL

Instrument Serial No. 008896 GREENSBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008896
Test Date: 02/09/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG035001
Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	11:01am
AIR BLK	.00	11:01am
ACCY CHK	.07	11:02am
AIR BLK	.00	11:03am
SUB TEST	.00	11:04am
AIR BLK	.00	11:05am
SUB TEST	.00	11:07am
AIR BLK	.00	11:08am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

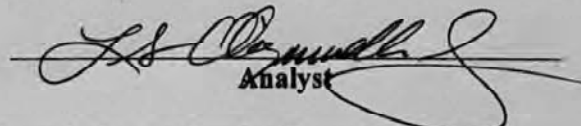
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

GUILFORD COUNTY GREENSBORO JAIL 400

Serial Number: 008896 Test Record Number: 1400
Test Date: 02/09/2021 Test Time: 11:08am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:09am
FLO	Pass	11:09am
FC	Pass	11:09am

Temperature Tests

Test	Status	Time
FC1	Pass	11:09am
SRC	Pass	11:09am
DET	Pass	11:09am
BAR	Pass	11:09am
BT	Pass	11:09am

Blank Tests

Test	Status	Time
AIR	Pass	11:10am


Printer Tests

Test	Status	Time
PRNT	Pass	11:10am

CRC Tests

Test	Status	Time
COMP	Pass	11:10am
CAL	Pass	11:10am

Preventive Maintenance
Status: Pass

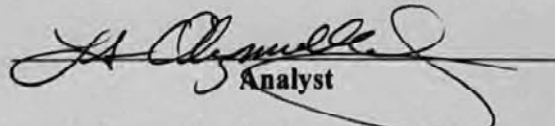
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Haywood Instrument Location Haywood Co. Jail
Instrument Serial No. 008714 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. Atch
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008714
Test Date: 02/25/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	10:18am
AIR BLK	.00	10:19am
ACCY CHK	.08	10:20am
AIR BLK	.00	10:21am
SUB TEST	.00	10:21am
AIR BLK	.00	10:22am
SUB TEST	.00	10:24am
AIR BLK	.00	10:25am

Reported AG: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008714 Test Record Number: 1758
Test Date: 02/25/2021 Test Time: 10:26am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:26am
FLO	Pass	10:26am
FC	Pass	10:26am

Temperature Tests

Test	Status	Time
FC1	Pass	10:26am
SRC	Pass	10:26am
DET	Pass	10:26am
BAR	Pass	10:26am
BT	Pass	10:26am

Blank Tests

Test	Status	Time
AIR	Pass	10:27am

Printer Tests

Test	Status	Time
PRNT	Pass	10:27am

CRC Tests

Test	Status	Time
COMP	Pass	10:27am
CAL	Pass	10:27am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Haywood Instrument Location Haywood Co. Jail
Instrument Serial No. 008911 Waynesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 11 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008911
Test Date: 02/11/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	10:47am
AIR BLK	.00	10:48am
ACCY CHK	.07	10:49am
AIR BLK	.00	10:50am
SUB TEST	.00	10:50am
AIR BLK	.00	10:51am
SUB TEST	.00	10:53am
AIR BLK	.00	10:54am

Reported AC: .00 g/210L

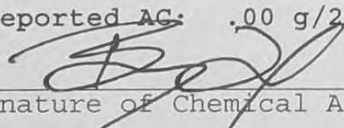
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

HAYWOOD COUNTY HAYWOOD COUNTY JAIL 430

Serial Number: 008911 Test Record Number: 653
Test Date: 02/11/2021 Test Time: 10:54am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:55am
FLO	Pass	10:55am
FC	Pass	10:55am

Temperature Tests

Test	Status	Time
FC1	Pass	10:55am
SRC	Pass	10:55am
DET	Pass	10:55am
BAR	Pass	10:55am
BT	Pass	10:55am

Blank Tests

Test	Status	Time
AIR	Pass	10:55am


Printer Tests

Test	Status	Time
PRNT	Pass	10:56am

CRC Tests

Test	Status	Time
COMP	Pass	10:56am
CAL	Pass	10:56am

Preventive Maintenance
Status: Pass

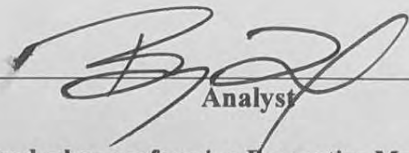
Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County JOHNSTON Instrument Location SELMA POLICE DEPT

Instrument Serial No. 008595

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 01 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Alan R. B...
Signature of Certifying Official

648
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595

Test Date: 02/01/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Alvin R

Permit Number: 0014-6279

Effective:

10/09/2020-10/09/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG911501

Exp Date: 04/25/2021


Test	g/210L	Time
DIAG	Pass	1:41pm
AIR BLK	.00	1:42pm
ACCY CHK	.07	1:43pm
AIR BLK	.00	1:44pm
SUB TEST	.00	1:45pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:47pm
AIR BLK	.00	1:48pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY SELMA PD 500

Serial Number: 008595 Test Record Number: 1510
Test Date: 02/01/2021 Test Time: 1:48pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:49pm
FLO	Pass	1:49pm
FC	Pass	1:49pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:49pm
SRC	Pass	1:49pm
DET	Pass	1:49pm
BAR	Pass	1:49pm
BT	Pass	1:49pm

Blank Tests

Test	Status	Time
AIR	Pass	1:49pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:49pm

CRC Tests

Test	Status	Time
COMP	Pass	1:50pm
CAL	Pass	1:50pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Jones Instrument Location Jones County
Instrument Serial No. 008705 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JONES COUNTY DETENTION CENTER 510

Serial Number: 008705
Test Date: 02/22/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022


Test	g/210L	Time
DIAG	Pass	1:01pm
AIR BLK	.00	1:02pm
ACCY CHK	.07	1:02pm
AIR BLK	.00	1:04pm
SUB TEST	.00	1:05pm
AIR BLK	.00	1:05pm
SUB TEST	.00	1:07pm
AIR BLK	.00	1:08pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

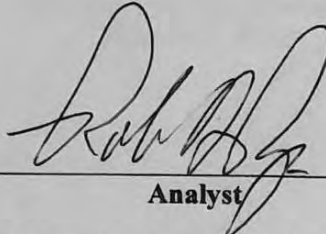

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

JONES COUNTY DETENTION CENTER 510

Serial Number: 008705 Test Record Number: 1497
Test Date: 02/22/2021 Test Time: 1:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:09pm
FLO	Pass	1:09pm
FC	Pass	1:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:10pm
SRC	Pass	1:10pm
DET	Pass	1:10pm
BAR	Pass	1:10pm
BT	Pass	1:10pm

Blank Tests

Test	Status	Time
AIR	Pass	1:10pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:10pm

CRC Tests

Test	Status	Time
COMP	Pass	1:10pm
CAL	Pass	1:10pm

Preventive Maintenance
Status: Pass

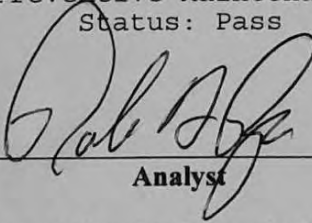

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County LEE Instrument Location SANFORD POLICE DEPT.
Instrument Serial No. 008867 SANFORD, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22ND day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

667

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867
Test Date: 02/22/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG934001

Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	4:18pm
AIR BLK	.00	4:18pm
ACCY CHK	.07	4:19pm
AIR BLK	.00	4:20pm
SUB TEST	.00	4:21pm
AIR BLK	.00	4:22pm
SUB TEST	.00	4:23pm
AIR BLK	.00	4:24pm

Reported AC: .00 g/210L

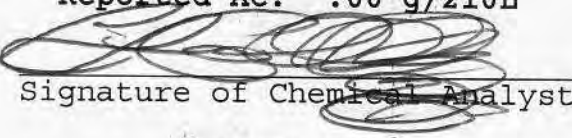
Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867 Test Record Number: 1214
Test Date: 02/22/2021 Test Time: 4:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:25pm
FLO	Pass	4:25pm
FC	Pass	4:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:25pm
SRC	Pass	4:25pm
DET	Pass	4:25pm
BAR	Pass	4:25pm
BT	Pass	4:25pm

Blank Tests

Test	Status	Time
AIR	Pass	4:26pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:26pm

CRC Tests

Test	Status	Time
COMP	Pass	4:26pm
CAL	Pass	4:26pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Lenoir Instrument Location Kinston P.D.

Instrument Serial No. 008624 205 E King St, Kinston, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY KINSTON PD 530

Serial Number: 008624

Test Date: 02/05/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021


Test	g/210L	Time
DIAG	Pass	2:38pm
AIR BLK	.00	2:39pm
ACCY CHK	.08	2:40pm
AIR BLK	.00	2:41pm
SUB TEST	.00	2:42pm
AIR BLK	.00	2:43pm
SUB TEST	.00	2:44pm
AIR BLK	.00	2:45pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY KINSTON PD 530

Serial Number: 008624 Test Record Number: 1916
Test Date: 02/05/2021 Test Time: 2:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:46pm
FLO	Pass	2:46pm
FC	Pass	2:46pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:46pm
SRC	Pass	2:46pm
DET	Pass	2:46pm
BAR	Pass	2:46pm
BT	Pass	2:46pm

Blank Tests

Test	Status	Time
AIR	Pass	2:47pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:47pm

CRC Tests

Test	Status	Time
COMP	Pass	2:47pm
CAL	Pass	2:47pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lenoir Instrument Location Lenoir, G.S.O.
Instrument Serial No. 009639 130 Queen St, Kingston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008639
Test Date: 02/05/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	2:12pm
AIR BLK	.00	2:13pm
ACCY CHK	.07	2:14pm
AIR BLK	.00	2:15pm
SUB TEST	.00	2:16pm
AIR BLK	.00	2:17pm
SUB TEST	.00	2:18pm
AIR BLK	.00	2:19pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

LENOIR COUNTY LENOIR CO SO 530

Serial Number: 008639 Test Record Number: 3519
Test Date: 02/05/2021 Test Time: 2:20pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:20pm
FLO	Pass	2:20pm
FC	Pass	2:20pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:20pm
SRC	Pass	2:20pm
DET	Pass	2:20pm
BAR	Pass	2:20pm
BT	Pass	2:20pm

Blank Tests

Test	Status	Time
AIR	Pass	2:21pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:21pm

CRC Tests

Test	Status	Time
COMP	Pass	2:21pm
CAL	Pass	2:21pm

Preventive Maintenance
Status: Pass

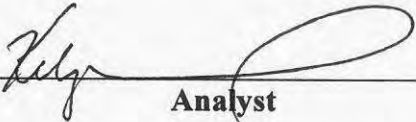

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Lincoln Instrument Location Lincoln County 50

Instrument Serial No. 008827 700 John Howell Memorial Drive
Lincolnton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827

Test Date: 02/24/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022


Test	g/210L	Time
DIAG	Pass	1:28pm
AIR BLK	.00	1:29pm
ACCY CHK	.08	1:29pm
AIR BLK	.00	1:31pm
SUB TEST	.00	1:31pm
AIR BLK	.00	1:32pm
SUB TEST	.00	1:34pm
AIR BLK	.00	1:34pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

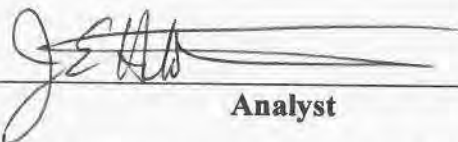

Analyst

Intox EC/IR-II: Preventive Maintenance

LINCOLN COUNTY LINCOLN COUNTY SO 540

Serial Number: 008827 Test Record Number: 3483
Test Date: 02/24/2021 Test Time: 1:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:36pm
FLO	Pass	1:36pm
FC	Pass	1:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:36pm
SRC	Pass	1:36pm
DET	Pass	1:36pm
BAR	Pass	1:36pm
BT	Pass	1:36pm

Blank Tests

Test	Status	Time
AIR	Pass	1:37pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:37pm

CRC Tests

Test	Status	Time
COMP	Pass	1:37pm
CAL	Pass	1:37pm

Preventive Maintenance
Status: Pass

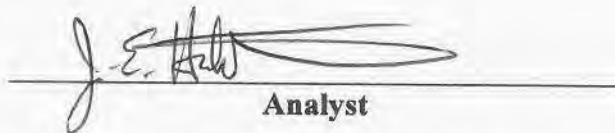
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Macon Instrument Location Macon County Jail
Instrument Serial No. 008618 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Paul R. [Signature]
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008618
Test Date: 02/10/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Cutler, Daniel R
Permit Number: 0084-3310
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG919901
Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	1:42pm
AIR BLK	.00	1:43pm
ACCY CHK	.07	1:44pm
AIR BLK	.00	1:45pm
SUB TEST	.00	1:45pm
AIR BLK	.00	1:46pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008618 Test Record Number: 2124
Test Date: 02/10/2021 Test Time: 1:50pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:50pm
FLO	Pass	1:50pm
FC	Pass	1:50pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:50pm
SRC	Pass	1:50pm
DET	Pass	1:50pm
BAR	Pass	1:50pm
BT	Pass	1:50pm

Blank Tests

Test	Status	Time
AIR	Pass	1:51pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:51pm

CRC Tests

Test	Status	Time
COMP	Pass	1:51pm
CAL	Pass	1:51pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Macon Instrument Location Macon Co. Jail

Instrument Serial No. 008789 Franklin, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Orville R. Carter
Signature of Certifying Official

635
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008789
Test Date: 02/10/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Cutler, Daniel R

Permit Number: 0084-3310

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG018801

Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	1:45pm
AIR BLK	.00	1:45pm
ACCY CHK	.07	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

MACON COUNTY MACON COUNTY JAIL 550

Serial Number: 008789 Test Record Number: 695
Test Date: 02/10/2021 Test Time: 1:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:52pm
FLO	Pass	1:52pm
FC	Pass	1:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:52pm
SRC	Pass	1:52pm
DET	Pass	1:52pm
BAR	Pass	1:52pm
BT	Pass	1:52pm

Blank Tests

Test	Status	Time
AIR	Pass	1:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:53pm

CRC Tests

Test	Status	Time
COMP	Pass	1:53pm
CAL	Pass	1:53pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County McDowell Instrument Location McDowell County Jail

Instrument Serial No. 009888 Moreau, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008888

Test Date: 02/24/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C

Permit Number: 0024-4987

Effective:

09/17/2020-09/17/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018801


Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	12:44pm
AIR BLK	.00	12:45pm
ACCY CHK	.07	12:46pm
AIR BLK	.00	12:47pm
SUB TEST	.00	12:48pm
AIR BLK	.00	12:49pm
SUB TEST	.00	12:50pm
AIR BLK	.00	12:51pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008888 Test Record Number: 1590
Test Date: 02/24/2021 Test Time: 12:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:53pm
FLO	Pass	12:53pm
FC	Pass	12:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:53pm
SRC	Pass	12:53pm
DET	Pass	12:53pm
BAR	Pass	12:53pm
BT	Pass	12:53pm

Blank Tests

Test	Status	Time
AIR	Pass	12:53pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:54pm

CRC Tests

Test	Status	Time
COMP	Pass	12:54pm
CAL	Pass	12:54pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County McDowell Instrument Location McDowell County Jail
Instrument Serial No. 008892 Morion, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MCDOWELL COUNTY JAIL 580

Serial Number: 008892
Test Date: 02/24/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:43pm
AIR BLK	.00	12:44pm
ACCY CHK	.07	12:45pm
AIR BLK	.00	12:46pm
SUB TEST	.00	12:47pm
AIR BLK	.00	12:48pm
SUB TEST	.00	12:49pm
AIR BLK	.00	12:50pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MCDOWELL COUNTY JAIL 580

Serial Number: 008892 Test Record Number: 943
Test Date: 02/24/2021 Test Time: 12:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:51pm
FLO	Pass	12:51pm
FC	Pass	12:51pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:51pm
SRC	Pass	12:51pm
DET	Pass	12:51pm
BAR	Pass	12:51pm
BT	Pass	12:51pm

Blank Tests

Test	Status	Time
AIR	Pass	12:52pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:52pm

CRC Tests

Test	Status	Time
COMP	Pass	12:52pm
CAL	Pass	12:52pm

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location CMPD LEC
Instrument Serial No. 008594 601 E. Trade Street, Charlotte

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Holt
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008594
Test Date: 02/26/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	12:07pm
AIR BLK	.00	12:08pm
ACCY CHK	.07	12:09pm
AIR BLK	.00	12:10pm
SUB TEST	.00	12:12pm
AIR BLK	.00	12:13pm
SUB TEST	.00	12:14pm
AIR BLK	.00	12:15pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

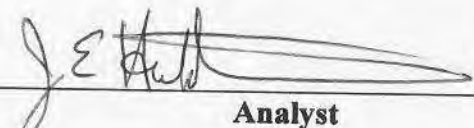

Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008594 Test Record Number: 4817
Test Date: 02/26/2021 Test Time: 12:16pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:16pm
FLO	Pass	12:16pm
FC	Pass	12:17pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:17pm
SRC	Pass	12:17pm
DET	Pass	12:17pm
BAR	Pass	12:17pm
BT	Pass	12:17pm

Blank Tests

Test	Status	Time
AIR	Pass	12:17pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:17pm

CRC Tests

Test	Status	Time
COMP	Pass	12:17pm
CAL	Pass	12:17pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Mecklenburg County SO
Instrument Serial No. 008665 801 E. 4th Street, Charlotte

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665

Test Date: 02/26/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG933901

Exp Date: 12/05/2021


Test	g/210L	Time
DIAG	Pass	12:49pm
AIR BLK	.00	12:50pm
ACCY CHK	.08	12:51pm
AIR BLK	.00	12:52pm
SUB TEST	.00	12:53pm
AIR BLK	.00	12:54pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

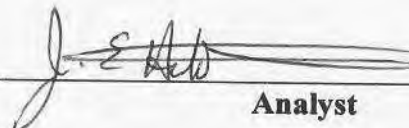

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008665 Test Record Number: 4924
Test Date: 02/26/2021 Test Time: 12:58pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:58pm
FLO	Pass	12:58pm
FC	Pass	12:59pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:59pm
SRC	Pass	12:59pm
DET	Pass	12:59pm
BAR	Pass	12:59pm
BT	Pass	12:59pm

Blank Tests

Test	Status	Time
AIR	Pass	12:59pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:59pm

CRC Tests

Test	Status	Time
COMP	Pass	12:59pm
CAL	Pass	12:59pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location Mecklenburg County SO
Instrument Serial No. 008690 801 E. 4th Street, Charlotte

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008690

Test Date: 02/26/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG934303

Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	12:42pm
AIR BLK	.00	12:43pm
ACCY CHK	.08	12:44pm
AIR BLK	.00	12:45pm
SUB TEST	.00	12:46pm
AIR BLK	.00	12:47pm
SUB TEST	.00	12:49pm
AIR BLK	.00	12:50pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY SHERIFFS OFFICE 590

Serial Number: 008690 Test Record Number: 6693
Test Date: 02/26/2021 Test Time: 12:51pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:52pm
FLO	Pass	12:52pm
FC	Pass	12:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:52pm
SRC	Pass	12:52pm
DET	Pass	12:52pm
BAR	Pass	12:52pm
BT	Pass	12:52pm

Blank Tests

Test	Status	Time
AIR	Pass	12:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:53pm

CRC Tests

Test	Status	Time
COMP	Pass	12:53pm
CAL	Pass	12:53pm

Preventive Maintenance
Status: Pass

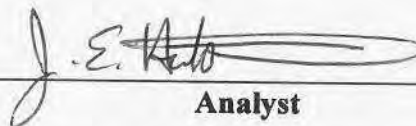

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Mecklenburg Instrument Location CMPD LEC

Instrument Serial No. 008691 601 E. Trade Street, Charlotte

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hight
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691

Test Date: 02/26/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034902


Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	12:08pm
AIR BLK	.00	12:09pm
ACCY CHK	.08	12:10pm
AIR BLK	.00	12:12pm
SUB TEST	.00	12:13pm
AIR BLK	.00	12:14pm
SUB TEST	.00	12:17pm
AIR BLK	.00	12:18pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

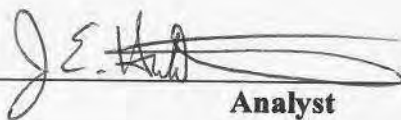
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008691 Test Record Number: 8341
Test Date: 02/26/2021 Test Time: 12:19pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:19pm
FLO	Pass	12:19pm
FC	Pass	12:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:19pm
SRC	Pass	12:19pm
DET	Pass	12:19pm
BAR	Pass	12:19pm
BT	Pass	12:19pm

Blank Tests

Test	Status	Time
AIR	Pass	12:20pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:20pm

CRC Tests

Test	Status	Time
COMP	Pass	12:20pm
CAL	Pass	12:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Pineville PD
Instrument Serial No. 008703 427 Main Street, Pineville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 19th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703

Test Date: 02/19/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	1:15pm
AIR BLK	.00	1:16pm
ACCY CHK	.08	1:17pm
AIR BLK	.00	1:18pm
SUB TEST	.00	1:18pm
AIR BLK	.00	1:19pm
SUB TEST	.00	1:21pm
AIR BLK	.00	1:22pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG COUNTY PINEVILLE PD 590

Serial Number: 008703 Test Record Number: 5918
Test Date: 02/19/2021 Test Time: 1:23pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:23pm
FLO	Pass	1:23pm
FC	Pass	1:23pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:24pm
SRC	Pass	1:24pm
DET	Pass	1:24pm
BAR	Pass	1:24pm
BT	Pass	1:24pm

Blank Tests

Test	Status	Time
AIR	Pass	1:24pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:24pm

CRC Tests

Test	Status	Time
COMP	Pass	1:24pm
CAL	Pass	1:24pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mecklenburg Instrument Location Huntersville PD

Instrument Serial No. 008747 9630 Julian Clark Ave,
Huntersville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: 008747

Test Date: 02/26/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	2:01pm
AIR BLK	.00	2:02pm
ACCY CHK	.08	2:03pm
AIR BLK	.00	2:04pm
SUB TEST	.00	2:04pm
AIR BLK	.00	2:06pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:08pm

Reported AC: .00 g/210L

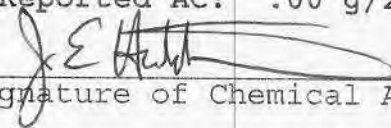

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG HUNTERSVILLE PD 590

Serial Number: 008747 Test Record Number: 2806
Test Date: 02/26/2021 Test Time: 2:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:13pm
FLO	Pass	2:13pm
FC	Pass	2:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:13pm
SRC	Pass	2:13pm
DET	Pass	2:13pm
BAR	Pass	2:13pm
BT	Pass	2:13pm

Blank Tests

Test	Status	Time
AIR	Pass	2:14pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:14pm

CRC Tests

Test	Status	Time
COMP	Pass	2:14pm
CAL	Pass	2:14pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Mitchell Instrument Location Spruce Pine PD

Instrument Serial No. 008911 Spruce Pine, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

668
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MITCHELL COUNTY SPRUCE PINE POLICE
DEPARTMENT 600

Serial Number: 008911
Test Date: 02/04/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Loftis, Benjamin C
Permit Number: 0024-4987
Effective:
09/17/2020-09/17/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG920301
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	9:47am
AIR BLK	.00	9:48am
ACCY CHK	.07	9:49am
AIR BLK	.00	9:50am
SUB TEST	.00	9:50am
AIR BLK	.00	9:51am
SUB TEST	.00	9:53am
AIR BLK	.00	9:53am

Reported AC: .00 g/210L

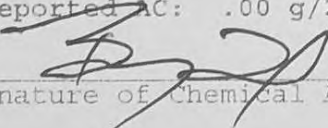

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

MITCHELL COUNTY SPRUCE PINE POLICE DEPARTMENT 600

Serial Number: 008911 Test Record Number: 649
Test Date: 02/04/2021 Test Time: 9:54am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	9:54am
FLO	Pass	9:54am
FC	Pass	9:54am

Temperature Tests

Test	Status	Time
FC1	Pass	9:54am
SRC	Pass	9:54am
DET	Pass	9:54am
BAR	Pass	9:54am
BT	Pass	9:54am

Blank Tests

Test	Status	Time
AIR	Pass	9:55am


Printer Tests

Test	Status	Time
PRNT	Pass	9:55am

CRC Tests

Test	Status	Time
COMP	Pass	9:55am
CAL	Pass	9:55am

Preventive Maintenance
Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County MONTGOMERY Instrument Location MONTGOMERY CO. DETENTION CENTER
Instrument Serial No. 008657 TROY, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4TH day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Signature of Certifying Official

667

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008657
Test Date: 02/04/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	7:26pm
AIR BLK	.00	7:27pm
ACCY CHK	.08	7:28pm
AIR BLK	.00	7:29pm
SUB TEST	.00	7:30pm
AIR BLK	.00	7:30pm
SUB TEST	.00	7:32pm
AIR BLK	.00	7:33pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008657 Test Record Number: 1792
Test Date: 02/04/2021 Test Time: 7:35pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:35pm
FLO	Pass	7:35pm
FC	Pass	7:35pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:35pm
SRC	Pass	7:35pm
DET	Pass	7:35pm
BAR	Pass	7:35pm
BT	Pass	7:35pm

Blank Tests

Test	Status	Time
AIR	Pass	7:36pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:36pm

CRC Tests

Test	Status	Time
COMP	Pass	7:36pm
CAL	Pass	7:36pm

Preventive Maintenance
Status: Pass

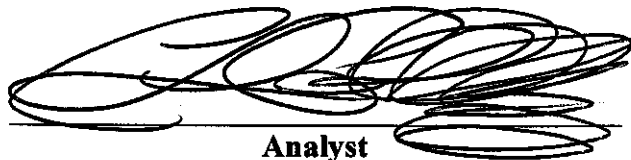
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County MONTGOMERY Instrument Location MONTGOMERY CO. DETENTION CENTER
Instrument Serial No. 008709 TROY, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4TH day of FEBRUARY, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008709
Test Date: 02/04/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG919902

Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	7:28pm
AIR BLK	.00	7:28pm
ACCY CHK	.07	7:29pm
AIR BLK	.00	7:30pm
SUB TEST	.00	7:31pm
AIR BLK	.00	7:32pm
SUB TEST	.00	7:33pm
AIR BLK	.00	7:35pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

MONTGOMERY COUNTY DETENTION CENTER 610

Serial Number: 008709 Test Record Number: 1252
Test Date: 02/04/2021 Test Time: 7:40pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	7:41pm
FLO	Pass	7:41pm
FC	Pass	7:41pm

Temperature Tests

Test	Status	Time
FC1	Pass	7:41pm
SRC	Pass	7:41pm
DET	Pass	7:41pm
BAR	Pass	7:41pm
BT	Pass	7:41pm

Blank Tests

Test	Status	Time
AIR	Pass	7:42pm


Printer Tests

Test	Status	Time
PRNT	Pass	7:42pm

CRC Tests

Test	Status	Time
COMP	Pass	7:42pm
CAL	Pass	7:42pm

Preventive Maintenance
Status: Pass

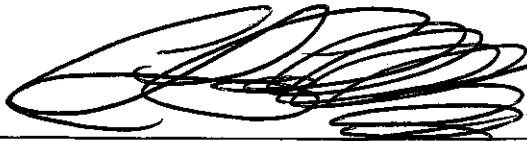

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location Onslow County
Instrument Serial No. 008819 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 300

Serial Number: 008819

Test Date: 02/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	1:25pm
AIR BLK	.00	1:26pm
ACCY CHK	.08	1:26pm
AIR BLK	.00	1:27pm
SUB TEST	.00	1:28pm
AIR BLK	.00	1:29pm
SUB TEST	.00	1:30pm
AIR BLK	.00	1:31pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 300

Serial Number: 008819 Test Record Number: 774
Test Date: 02/02/2021 Test Time: 1:34pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:34pm
FLO	Pass	1:34pm
FC	Pass	1:34pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:34pm
SRC	Pass	1:34pm
DET	Pass	1:34pm
BAR	Pass	1:34pm
BT	Pass	1:34pm

Blank Tests

Test	Status	Time
AIR	Pass	1:35pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:35pm

CRC Tests

Test	Status	Time
COMP	Pass	1:35pm
CAL	Pass	1:35pm

Preventive Maintenance
Status: *Pass*

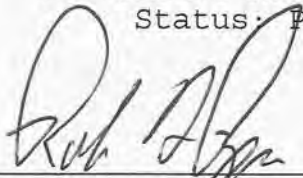

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location Onslow County
Instrument Serial No. 008819 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Robert P. [Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008819
Test Date: 02/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	9:51am
AIR BLK	.00	9:52am
ACCY CHK	.08	9:52am
AIR BLK	.00	9:53am
SUB TEST	.00	9:54am
AIR BLK	.00	9:55am
SUB TEST	.00	9:56am
AIR BLK	.00	9:57am

Reported AC: .00 g/210L

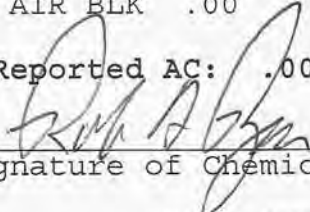

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008819 Test Record Number: 779
Test Date: 02/03/2021 Test Time: 10:00am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:00am
FLO	Pass	10:00am
FC	Pass	10:00am

Temperature Tests

Test	Status	Time
FC1	Pass	10:00am
SRC	Pass	10:00am
DET	Pass	10:00am
BAR	Pass	10:00am
BT	Pass	10:00am

Blank Tests

Test	Status	Time
AIR	Pass	10:01am


Printer Tests

Test	Status	Time
PRNT	Pass	10:01am

CRC Tests

Test	Status	Time
COMP	Pass	10:01am
CAL	Pass	10:01am

Preventive Maintenance
Status: *Pass*

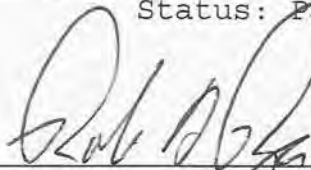

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location Onslow County
Instrument Serial No. 008917 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Robert D. [Signature] 670
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008917

Test Date: 02/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	9:53am
AIR BLK	.00	9:54am
ACCY CHK	.07	9:54am
AIR BLK	.00	9:56am
SUB TEST	.00	9:57am
AIR BLK	.00	9:57am
SUB TEST	.00	9:59am
AIR BLK	.00	10:00am

Reported AC: .00 g/210L

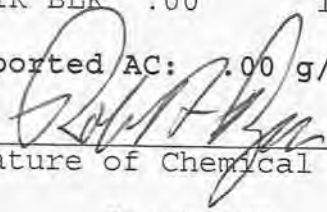

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008917 Test Record Number: 889
Test Date: 02/03/2021 Test Time: 10:02am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:02am
FLO	Pass	10:02am
FC	Pass	10:02am

Temperature Tests

Test	Status	Time
FC1	Pass	10:02am
SRC	Pass	10:02am
DET	Pass	10:02am
BAR	Pass	10:02am
BT	Pass	10:02am

Blank Tests

Test	Status	Time
AIR	Pass	10:03am


Printer Tests

Test	Status	Time
PRNT	Pass	10:03am

CRC Tests

Test	Status	Time
COMP	Pass	10:03am
CAL	Pass	10:03am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location MCAS New River

Instrument Serial No. 008919 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919
Test Date: 02/05/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:33pm
AIR BLK	.00	12:34pm
ACCY CHK	.07	12:34pm
AIR BLK	.00	12:36pm
SUB TEST	.00	12:36pm
AIR BLK	.00	12:37pm
SUB TEST	.00	12:39pm
AIR BLK	.00	12:40pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY MCAS NEW RIVER 660

Serial Number: 008919 Test Record Number: 712
Test Date: 02/05/2021 Test Time: 12:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:42pm
FLO	Pass	12:42pm
FC	Pass	12:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:42pm
SRC	Pass	12:42pm
DET	Pass	12:42pm
BAR	Pass	12:42pm
BT	Pass	12:42pm

Blank Tests

Test	Status	Time
AIR	Pass	12:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:43pm

CRC Tests

Test	Status	Time
COMP	Pass	12:43pm
CAL	Pass	12:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location Camp LeJeune
Instrument Serial No. 008922 PMO

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Robert [Signature] Signature of Certifying Official 670 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008922
Test Date: 02/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018801
Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	3:03pm
AIR BLK	.00	3:04pm
ACCY CHK	.08	3:04pm
AIR BLK	.00	3:05pm
SUB TEST	.00	3:06pm
AIR BLK	.00	3:07pm
SUB TEST	.00	3:09pm
AIR BLK	.00	3:10pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY CAMP LEJEUNE PMO 660

Serial Number: 008922 Test Record Number: 405
Test Date: 02/03/2021 Test Time: 3:11pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:12pm
FLO	Pass	3:12pm
FC	Pass	3:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:12pm
SRC	Pass	3:12pm
DET	Pass	3:12pm
BAR	Pass	3:12pm
BT	Pass	3:12pm

Blank Tests

Test	Status	Time
AIR	Pass	3:12pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:13pm

CRC Tests

Test	Status	Time
COMP	Pass	3:13pm
CAL	Pass	3:13pm

Preventive Maintenance
Status: *Pass*



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location Jacksonville

Instrument Serial No. 008930 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Inbox EC/IR-II: Subject Test

ONSELOW COUNTY JACKSONVILLE PD 660

Serial Number: 008930

Test Date: 02/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG018801


Exp Date: 07/06/2022

Test	g/210L	Time
DIAG	Pass	3:06pm
AIR BLK	.00	3:07pm
ACCY CHK	.08	3:07pm
AIR BLK	.00	3:08pm
SUB TEST	.00	3:09pm
AIR BLK	.00	3:10pm
SUB TEST	.00	3:11pm
AIR BLK	.00	3:12pm

Reported AC1 .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY JACKSONVILLE PD 660

Serial Number: 008930 Test Record Number: 2097
Test Date: 02/02/2021 Test Time: 3:14pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:14pm
FLO	Pass	3:14pm
FC	Pass	3:14pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:14pm
SRC	Pass	3:14pm
DET	Pass	3:14pm
BAR	Pass	3:14pm
BT	Pass	3:14pm

Blank Tests

Test	Status	Time
AIR	Pass	3:15pm

Printer Tests


Test	Status	Time
PRNT	Pass	3:15pm

CRC Tests

Test	Status	Time
COMP	Pass	3:15pm
CAL	Pass	3:15pm

Preventive Maintenance

Status: Pass

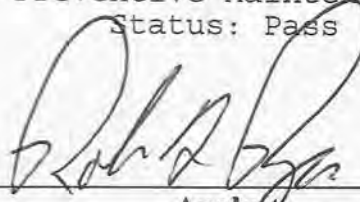

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Onslow Instrument Location Onslow County
Instrument Serial No. 008931 Detention Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931
Test Date: 02/18/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901

Exp Date: 12/14/2022


Test	g/210L	Time
DIAG	Pass	11:43am
AIR BLK	.00	11:43am
ACCY CHK	.08	11:44am
AIR BLK	.00	11:45am
SUB TEST	.00	11:47am
AIR BLK	.00	11:48am
SUB TEST	.00	11:49am
AIR BLK	.00	11:50am

Reported AC: .00 g/210L

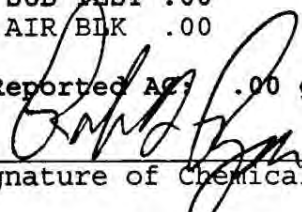

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONSLOW COUNTY DETENTION CENTER 660

Serial Number: 008931 Test Record Number: 3476
Test Date: 02/18/2021 Test Time: 11:59am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:00pm
FLO	Pass	12:00pm
FC	Pass	12:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:00pm
SRC	Pass	12:00pm
DET	Pass	12:00pm
BAR	Pass	12:00pm
BT	Pass	12:00pm

Blank Tests

Test	Status	Time
AIR	Pass	12:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:01pm

CRC Tests

Test	Status	Time
COMP	Pass	12:01pm
CAL	Pass	12:01pm

Preventive Maintenance
Status: Pass

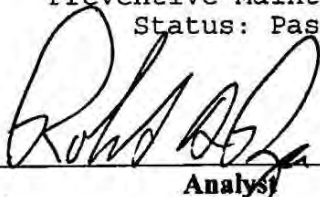

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Onslow Instrument Location Onslow County
Instrument Serial No. 008932 Detection Center

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 18th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

670
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008932
Test Date: 02/18/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034901
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	11:56am
AIR BLK	.00	11:57am
ACCY CHK	.08	11:57am
AIR BLK	.00	11:58am
SUB TEST	.00	11:59am
AIR BLK	.00	12:00pm
SUB TEST	.00	12:01pm
AIR BLK	.00	12:02pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ONslow COUNTY DETENTION CENTER 660

Serial Number: 008932 Test Record Number: 5947
Test Date: 02/18/2021 Test Time: 12:05pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:06pm
FLO	Pass	12:06pm
FC	Pass	12:06pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:06pm
SRC	Pass	12:06pm
DET	Pass	12:06pm
BAR	Pass	12:06pm
BT	Pass	12:06pm

Blank Tests

Test	Status	Time
AIR	Pass	12:07pm

Printer Tests


Test	Status	Time
PRNT	Pass	12:07pm

CRC Tests

Test	Status	Time
COMP	Pass	12:07pm
CAL	Pass	12:07pm

Preventive Maintenance

Status: Pass

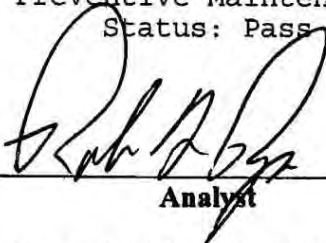

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ORANGE Instrument Location CARRBORO PD

Instrument Serial No. 008873 100 W. GREENSTOWN ST. CARRBORO, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

642
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008873

Test Date: 02/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Barnes, Simon S

Permit Number: 0014-6221

Effective:

09/01/2020-09/01/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG034901


Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	11:13am
AIR BLK	.00	11:14am
ACCY CHK	.08	11:14am
AIR BLK	.00	11:15am
SUB TEST	.00	11:16am
AIR BLK	.00	11:17am
SUB TEST	.00	11:18am
AIR BLK	.00	11:19am

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ORANGE COUNTY CARRBORO PD 670

Serial Number: 008873 Test Record Number: 1905
Test Date: 02/03/2021 Test Time: 11:20am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:20am
FLO	Pass	11:20am
FC	Pass	11:20am

Temperature Tests

Test	Status	Time
FC1	Pass	11:20am
SRC	Pass	11:20am
DET	Pass	11:20am
BAR	Pass	11:20am
BT	Pass	11:20am

Blank Tests

Test	Status	Time
AIR	Pass	11:21am


Printer Tests

Test	Status	Time
PRNT	Pass	11:21am

CRC Tests

Test	Status	Time
COMP	Pass	11:21am
CAL	Pass	11:21am

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County RANDOLPH Instrument Location RANDLEMAN POLICE DEPT.
Instrument Serial No. 008737 RANDLEMAN, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1ST day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



A large, stylized handwritten signature in black ink.

Signature of Certifying-Official

667

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: 008737

Test Date: 02/01/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Galloway, Charles L

Permit Number: 0023-9771

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG934001

Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	4:44pm
AIR BLK	.00	4:45pm
ACCY CHK	.08	4:46pm
AIR BLK	.00	4:47pm
SUB TEST	.00	4:47pm
AIR BLK	.00	4:48pm
SUB TEST	.00	4:50pm
AIR BLK	.00	4:50pm

Reported AC: .00 g/210L


Signature of ~~Chemical~~ Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: 008737 Test Record Number: 1213
Test Date: 02/01/2021 Test Time: 4:52pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:52pm
FLO	Pass	4:52pm
FC	Pass	4:52pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:52pm
SRC	Pass	4:52pm
DET	Pass	4:52pm
BAR	Pass	4:52pm
BT	Pass	4:52pm

Blank Tests

Test	Status	Time
AIR	Pass	4:53pm


Printer Tests

Test	Status	Time
PRNT	Pass	4:53pm

CRC Tests

Test	Status	Time
COMP	Pass	4:53pm
CAL	Pass	4:53pm

Preventive Maintenance
Status: Pass

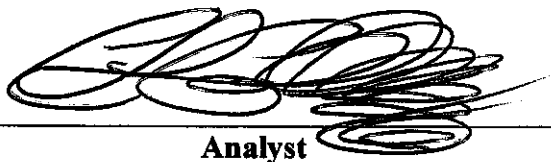

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County RANDOLPH Instrument Location ARCHDALE POLICE DEPT.
Instrument Serial No. 008791 ARCHDALE, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1ST day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1607
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY ARCHDALE PD 750

Serial Number: 008791
Test Date: 02/01/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933703
Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	3:26pm
AIR BLK	.00	3:26pm
ACCY CHK	.08	3:27pm
AIR BLK	.00	3:28pm
SUB TEST	.00	3:29pm
AIR BLK	.00	3:30pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:32pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY ARCHDALE PD 750

Serial Number: 008791 Test Record Number: 1432
Test Date: 02/01/2021 Test Time: 3:41pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:41pm
FLO	Pass	3:41pm
FC	Pass	3:42pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:42pm
SRC	Pass	3:42pm
DET	Pass	3:42pm
BAR	Pass	3:42pm
BT	Pass	3:42pm

Blank Tests

Test	Status	Time
AIR	Pass	3:42pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:42pm

CRC Tests

Test	Status	Time
COMP	Pass	3:43pm
CAL	Pass	3:43pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County RANDOLPH Instrument Location LIBERTY POLICE DEPT.
Instrument Serial No. 008830 LIBERTY, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 1ST day of FEBRUARY, 20 01 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830
Test Date: 02/01/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	6:01pm
AIR BLK	.00	6:02pm
ACCY CHK	.08	6:02pm
AIR BLK	.00	6:03pm
SUB TEST	.00	6:05pm
AIR BLK	.00	6:06pm
SUB TEST	.00	6:07pm
AIR BLK	.00	6:08pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

RANDOLPH COUNTY LIBERTY PD 750

Serial Number: 008830 Test Record Number: 699
Test Date: 02/01/2021 Test Time: 6:09pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	6:09pm
FLO	Pass	6:09pm
FC	Pass	6:10pm

Temperature Tests

Test	Status	Time
FC1	Pass	6:10pm
SRC	Pass	6:10pm
DET	Pass	6:10pm
BAR	Pass	6:10pm
BT	Pass	6:10pm

Blank Tests

Test	Status	Time
AIR	Pass	6:10pm

Printer Tests

Test	Status	Time
PRNT	Pass	6:10pm

CRC Tests

Test	Status	Time
COMP	Pass	6:11pm
CAL	Pass	6:11pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROBESON Instrument Location ST. PAULS POLICE DEPT.
Instrument Serial No. 008814 ST. PAULS, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23RD day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY ST PAULS PD 770

Serial Number: 008814
Test Date: 02/23/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	10:21am
AIR BLK	.00	10:22am
ACCY CHK	.08	10:23am
AIR BLK	.00	10:24am
SUB TEST	.00	10:25am
AIR BLK	.00	10:26am
SUB TEST	.00	10:28am
AIR BLK	.00	10:28am

Reported AC: .00 g/210L

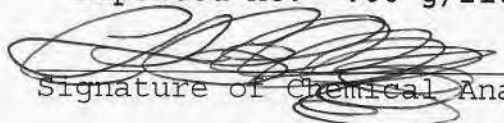
Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY ST PAULS PD 770

Serial Number: 008814 Test Record Number: 733
Test Date: 02/23/2021 Test Time: 10:30am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	10:30am
FLO	Pass	10:30am
FC	Pass	10:30am

Temperature Tests

Test	Status	Time
FC1	Pass	10:30am
SRC	Pass	10:30am
DET	Pass	10:30am
BAR	Pass	10:30am
BT	Pass	10:30am

Blank Tests

Test	Status	Time
AIR	Pass	10:31am


Printer Tests

Test	Status	Time
PRNT	Pass	10:31am

CRC Tests

Test	Status	Time
COMP	Pass	10:31am
CAL	Pass	10:31am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROBESON Instrument Location PEMBROKE POLICE DEPT.
Instrument Serial No. 008837 PEMBROKE, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23RD day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]
Signature of Certifying Official

667
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROBESON COUNTY PEMBROKE POLICE DEPT
770

Serial Number: 008837
Test Date: 02/23/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Galloway, Charles L
Permit Number: 0023-9771
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	2:10pm
AIR BLK	.00	2:10pm
ACCY CHK	.08	2:11pm
AIR BLK	.00	2:12pm
SUB TEST	.00	2:13pm
AIR BLK	.00	2:14pm
SUB TEST	.00	2:15pm
AIR BLK	.00	2:16pm

Reported AC: .00 g/210L


Signature of ~~Chemical~~ Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROBESON COUNTY PEMBROKE POLICE DEPT 770

Serial Number: 008837 Test Record Number: 1095
Test Date: 02/23/2021 Test Time: 2:17pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:18pm
FLO	Pass	2:18pm
FC	Pass	2:18pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:18pm
SRC	Pass	2:18pm
DET	Pass	2:18pm
BAR	Pass	2:18pm
BT	Pass	2:18pm

Blank Tests

Test	Status	Time
AIR	Pass	2:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:19pm

CRC Tests

Test	Status	Time
COMP	Pass	2:19pm
CAL	Pass	2:19pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROWAN Instrument Location SALISBURY

Instrument Serial No. 008835 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835

Test Date: 02/15/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG933703


Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	12:03pm
AIR BLK	.00	12:04pm
ACCY CHK	.08	12:04pm
AIR BLK	.00	12:06pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:08pm
SUB TEST	.00	12:09pm
AIR BLK	.00	12:10pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008835 Test Record Number: 2709
Test Date: 02/15/2021 Test Time: 12:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:12pm
FLO	Pass	12:12pm
FC	Pass	12:13pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:13pm
SRC	Pass	12:13pm
DET	Pass	12:13pm
BAR	Pass	12:13pm
BT	Pass	12:13pm

Blank Tests

Test	Status	Time
AIR	Pass	12:13pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:13pm

CRC Tests

Test	Status	Time
COMP	Pass	12:14pm
CAL	Pass	12:14pm

Preventive Maintenance
Status: Pass

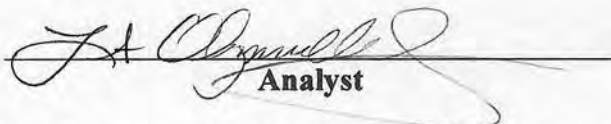
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County ROWAN Instrument Location CHINA GROVE
Instrument Serial No. 008862 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862
Test Date: 02/15/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Oligmueller Jr., Leo A
Permit Number: 0035-3799
Effective:
08/04/2020-08/04/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG821401
Exp Date: 07/22/2021

Test	g/210L	Time
DIAG	Pass	2:21pm
AIR BLK	.00	2:22pm
ACCY CHK	.08	2:22pm
AIR BLK	.00	2:24pm
SUB TEST	.00	2:24pm
AIR BLK	.00	2:25pm
SUB TEST	.00	2:27pm
AIR BLK	.00	2:28pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR

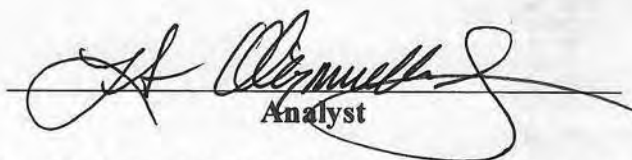
Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY CHINA GROVE PD 790

Serial Number: 008862 Test Record Number: 942
Test Date: 02/15/2021 Test Time: 2:29pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:30pm
FLO	Pass	2:30pm
FC	Pass	2:30pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:30pm
SRC	Pass	2:30pm
DET	Pass	2:30pm
BAR	Pass	2:30pm
BT	Pass	2:30pm

Blank Tests

Test	Status	Time
AIR	Pass	2:31pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:31pm

CRC Tests

Test	Status	Time
COMP	Pass	2:31pm
CAL	Pass	2:31pm

Preventive Maintenance
Status: Pass

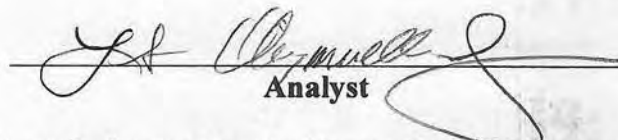
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County ROWAN Instrument Location SALISBURY

Instrument Serial No. 008868 POLICE DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 15 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

6669
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868

Test Date: 02/15/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG933703

Exp Date: 12/03/2021

Test	g/210L	Time
DIAG	Pass	12:04pm
AIR BLK	.00	12:05pm
ACCY CHK	.08	12:05pm
AIR BLK	.00	12:06pm
SUB TEST	.00	12:07pm
AIR BLK	.00	12:08pm
SUB TEST	.00	12:09pm
AIR BLK	.00	12:10pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

ROWAN COUNTY SALISBURY PD 790

Serial Number: 008868 Test Record Number: 3158
Test Date: 02/15/2021 Test Time: 12:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:12pm
FLO	Pass	12:12pm
FC	Pass	12:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:13pm
SRC	Pass	12:13pm
DET	Pass	12:13pm
BAR	Pass	12:13pm
BT	Pass	12:13pm

Blank Tests

Test	Status	Time
AIR	Pass	12:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:13pm

CRC Tests

Test	Status	Time
COMP	Pass	12:13pm
CAL	Pass	12:13pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**


County Scotland Instrument Location Laurinburg Police Department

Instrument Serial No. 008834

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SCOTLAND COUNTY LAURINBURG PD 820

Serial Number: 008834
Test Date: 02/08/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Ryan, Robert F
Permit Number: 0084-5023
Effective:
07/31/2020-07/31/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG934001
Exp Date: 12/06/2021

Test	g/210L	Time
DIAG	Pass	10:52am
AIR BLK	.00	10:53am
ACCY CHK	.08	10:53am
AIR BLK	.00	10:55am
SUB TEST	.00	10:55am
AIR BLK	.00	10:56am
SUB TEST	.00	10:58am
AIR BLK	.00	10:59am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SCOTLAND COUNTY LAURINBURG PD 820

Serial Number: 008834 Test Record Number: 996
Test Date: 02/08/2021 Test Time: 11:00am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:00am
FLO	Pass	11:00am
FC	Pass	11:00am

Temperature Tests

Test	Status	Time
FC1	Pass	11:00am
SRC	Pass	11:00am
DET	Pass	11:00am
BAR	Pass	11:00am
BT	Pass	11:00am

Blank Tests

Test	Status	Time
AIR	Pass	11:01am


Printer Tests

Test	Status	Time
PRNT	Pass	11:01am

CRC Tests

Test	Status	Time
COMP	Pass	11:01am
CAL	Pass	11:01am

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Scotland Instrument Location Scotland County
Instrument Serial No. 008861 Sheriff's Office

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

670

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SCOTLAND COUNTY SHERIFF'S OFFICE 820

Serial Number: 008861
Test Date: 02/08/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Ryan, Robert F

Permit Number: 0084-5023

Effective:

07/31/2020-07/31/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	11:35am
AIR BLK	.00	11:36am
ACCY CHK	.08	11:37am
AIR BLK	.00	11:38am
SUB TEST	.00	11:39am
AIR BLK	.00	11:40am
SUB TEST	.00	11:41am
AIR BLK	.00	11:42am

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SCOTLAND COUNTY SHERIFF'S OFFICE 820

Serial Number: 008861 Test Record Number: 1710
Test Date: 02/08/2021 Test Time: 11:43am EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	11:43am
FLO	Pass	11:43am
FC	Pass	11:44am

Temperature Tests

Test	Status	Time
FC1	Pass	11:44am
SRC	Pass	11:44am
DET	Pass	11:44am
BAR	Pass	11:44am
BT	Pass	11:44am

Blank Tests

Test	Status	Time
AIR	Pass	11:44am


Printer Tests

Test	Status	Time
PRNT	Pass	11:44am

CRC Tests

Test	Status	Time
COMP	Pass	11:44am
CAL	Pass	11:44am

Preventive Maintenance
Status: *Pass*

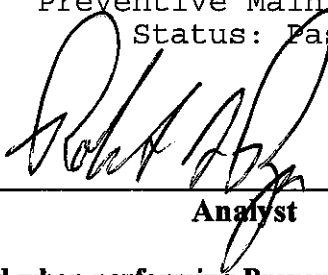

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Stanly Instrument Location Stanly Co 50

Instrument Serial No. 008824 126 S. 3rd Street, Albemarle

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 5th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hill
Signature of Certifying Official

654
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008824

Test Date: 02/05/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG919901

Exp Date: 07/18/2021


Test	g/210L	Time
DIAG	Pass	2:45pm
AIR BLK	.00	2:46pm
ACCY CHK	.08	2:47pm
AIR BLK	.00	2:48pm
SUB TEST	.00	2:49pm
AIR BLK	.00	2:50pm
SUB TEST	.00	2:51pm
AIR BLK	.00	2:52pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR

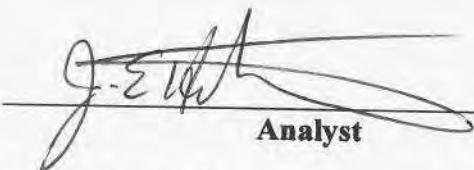

Analyst

Intox EC/IR-II: Preventive Maintenance

STANLY COUNTY STANLY COUNTY SO 830

Serial Number: 008824 Test Record Number: 1712
Test Date: 02/05/2021 Test Time: 2:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:53pm
FLO	Pass	2:53pm
FC	Pass	2:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:54pm
SRC	Pass	2:54pm
DET	Pass	2:54pm
BAR	Pass	2:54pm
BT	Pass	2:54pm

Blank Tests

Test	Status	Time
AIR	Pass	2:54pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:54pm

CRC Tests

Test	Status	Time
COMP	Pass	2:54pm
CAL	Pass	2:54pm

Preventive Maintenance
Status: Pass


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County STOKES Instrument Location KING POLICE

Instrument Serial No. 008718 DEPARTMENT

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 4 day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 669 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

STOKES COUNTY KING P D 840

Serial Number: 008718

Test Date: 02/04/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Oligmueller Jr., Leo A

Permit Number: 0035-3799

Effective:

08/04/2020-08/04/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	12:27pm
AIR BLK	.00	12:28pm
ACCY CHK	.07	12:28pm
AIR BLK	.00	12:30pm
SUB TEST	.00	12:30pm
AIR BLK	.00	12:31pm
SUB TEST	.00	12:33pm
AIR BLK	.00	12:33pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

STOKES COUNTY KING P D 840

Serial Number: 008718 Test Record Number: 2090
Test Date: 02/04/2021 Test Time: 12:36pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:36pm
FLO	Pass	12:36pm
FC	Pass	12:36pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:36pm
SRC	Pass	12:36pm
DET	Pass	12:36pm
BAR	Pass	12:36pm
BT	Pass	12:36pm

Blank Tests

Test	Status	Time
AIR	Pass	12:37pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:37pm

CRC Tests

Test	Status	Time
COMP	Pass	12:37pm
CAL	Pass	12:37pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Surry Instrument Location Mount Airy
Instrument Serial No. 008943 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 24 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943
Test Date: 02/24/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG007601


Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:47pm
AIR BLK	.00	1:48pm
ACCY CHK	.07	1:49pm
AIR BLK	.00	1:50pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm
SUB TEST	.00	1:53pm
AIR BLK	.00	1:54pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

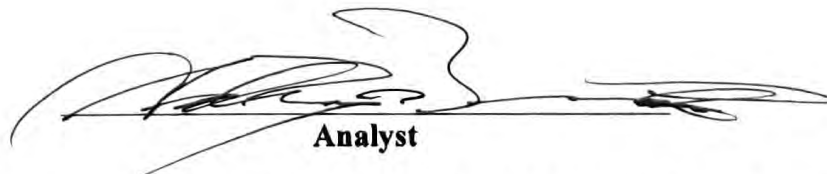

Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

SURRY COUNTY MOUNT AIRY PD 850

Serial Number: 008943 Test Record Number: 2281
Test Date: 02/24/2021 Test Time: 1:54pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:55pm
FLO	Pass	1:55pm
FC	Pass	1:55pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:55pm
SRC	Pass	1:55pm
DET	Pass	1:55pm
BAR	Pass	1:55pm
BT	Pass	1:55pm

Blank Tests

Test	Status	Time
AIR	Pass	1:56pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:56pm

CRC Tests

Test	Status	Time
COMP	Pass	1:56pm
CAL	Pass	1:56pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Union Instrument Location Stallings PD

Instrument Serial No. 008694 315 Stallings Rd, Stallings

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12th day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joyce E. Helton
Signature of Certifying Official

650
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

UNION COUNTY STALLINGS PD 890

Serial Number: 008694

Test Date: 02/12/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Hutchinson, Joseph E

Permit Number: 0035-6075

Effective:

10/13/2020-10/13/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG035001

Exp Date: 12/15/2022


Test	g/210L	Time
DIAG	Pass	4:18pm
AIR BLK	.00	4:19pm
ACCY CHK	.08	4:19pm
AIR BLK	.00	4:20pm
SUB TEST	.00	4:21pm
AIR BLK	.00	4:22pm
SUB TEST	.00	4:23pm
AIR BLK	.00	4:24pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

UNION COUNTY STALLINGS PD 890

Serial Number: 008694 Test Record Number: 1516
Test Date: 02/12/2021 Test Time: 4:25pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	4:25pm
FLO	Pass	4:25pm
FC	Pass	4:25pm

Temperature Tests

Test	Status	Time
FC1	Pass	4:26pm
SRC	Pass	4:26pm
DET	Pass	4:26pm
BAR	Pass	4:26pm
BT	Pass	4:26pm

Blank Tests

Test	Status	Time
AIR	Pass	4:26pm

Printer Tests

Test	Status	Time
PRNT	Pass	4:26pm

CRC Tests

Test	Status	Time
COMP	Pass	4:26pm
CAL	Pass	4:26pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Cary P.D.
Instrument Serial No. 008587 120 Wilkerson Ave
Cary, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



E.A. Brantley

Signature of Certifying Official

671

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY CARY PD 910

Serial Number: 008587
Test Date: 02/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG034902

Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	3:30pm
AIR BLK	.00	3:31pm
ACCY CHK	.07	3:31pm
AIR BLK	.00	3:33pm
SUB TEST	.00	3:33pm
AIR BLK	.00	3:34pm
SUB TEST	.00	3:36pm
AIR BLK	.00	3:37pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY CARY PD 910

Serial Number: 008587 Test Record Number: 4423
Test Date: 02/02/2021 Test Time: 3:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:38pm
FLO	Pass	3:38pm
FC	Pass	3:38pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:38pm
SRC	Pass	3:38pm
DET	Pass	3:38pm
BAR	Pass	3:38pm
BT	Pass	3:38pm

Blank Tests

Test	Status	Time
AIR	Pass	3:39pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:39pm

CRC Tests

Test	Status	Time
COMP	Pass	3:39pm
CAL	Pass	3:39pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Wake Co Detention Ctr
Instrument Serial No. 008012 3301 Hammond Rd Raleigh NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 667
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008612
Test Date: 02/12/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
09/01/2020-09/01/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test


Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	3:27pm
AIR BLK	.00	3:28pm
ACCY CHK	.08	3:29pm
AIR BLK	.00	3:30pm
SUB TEST	.00	3:31pm
AIR BLK	.00	3:32pm
SUB TEST	.00	3:34pm
AIR BLK	.00	3:35pm

Reported AG: .00 g/210L


Signature of Chemical Analyst

Court CVR

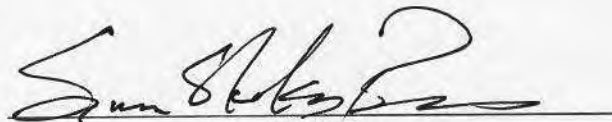
Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 310

Serial Number: 008612 Test Record Number: 4642
Test Date: 02/12/2021 Test Time: 3:38pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:39pm
FLO	Pass	3:39pm
FC	Pass	3:39pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:39pm
SRC	Pass	3:39pm
DET	Pass	3:39pm
BAR	Pass	3:39pm
BT	Pass	3:39pm

Blank Tests

Test	Status	Time
AIR	Pass	3:40pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:40pm

CRC Tests

Test	Status	Time
COMP	Pass	3:40pm
CAL	Pass	3:40pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wake Instrument Location Apex PD Station 4

Instrument Serial No. 008621 1615 E Williams St
Apex, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Eda Smith Signature of Certifying Official 671 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY APEX PD

Serial Number: 008621
Test Date: 02/02/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG919902

Exp Date: 07/18/2021

Test	g/210L	Time
DIAG	Pass	4:53pm
AIR BLK	.00	4:54pm
ACCY CHK	.07	4:55pm
AIR BLK	.00	4:56pm
SUB TEST	.00	4:56pm
AIR BLK	.00	4:57pm
SUB TEST	.00	4:59pm
AIR BLK	.00	5:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY APEX PD

Serial Number: 008621 Test Record Number: 2942
Test Date: 02/02/2021 Test Time: 5:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	5:01pm
FLO	Pass	5:01pm
FC	Pass	5:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	5:01pm
SRC	Pass	5:01pm
DET	Pass	5:01pm
BAR	Pass	5:01pm
BT	Pass	5:01pm

Blank Tests

Test	Status	Time
AIR	Pass	5:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	5:01pm

CRC Tests

Test	Status	Time
COMP	Pass	5:02pm
CAL	Pass	5:02pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Forest PD
Instrument Serial No. 108700 225 S Taylor St
Wake Forest, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31 day of February, 20 21 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



EAB
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY WAKE FOREST PD 910

Serial Number: 008700
Test Date: 02/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Bryant Jr., Earl A

Permit Number: 0017-9707

Effective:

09/15/2020-09/15/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG934303


Exp Date: 12/09/2021

Test	g/210L	Time
DIAG	Pass	12:11pm
AIR BLK	.00	12:12pm
ACCY CHK	.08	12:12pm
AIR BLK	.00	12:14pm
SUB TEST	.00	12:14pm
AIR BLK	.00	12:15pm
SUB TEST	.00	12:17pm
AIR BLK	.00	12:17pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY WAKE FOREST PD 910

Serial Number: 008700 Test Record Number: 1798
Test Date: 02/03/2021 Test Time: 12:18pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:19pm
FLO	Pass	12:19pm
FC	Pass	12:19pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:19pm
SRC	Pass	12:19pm
DET	Pass	12:19pm
BAR	Pass	12:19pm
BT	Pass	12:19pm

Blank Tests

Test	Status	Time
AIR	Pass	12:19pm

Printer Tests

Test	Status	Time
PRNT	Pass	12:19pm

CRC Tests

Test	Status	Time
COMP	Pass	12:20pm
CAL	Pass	12:20pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Knightdale PD

Instrument Serial No. 008838 879 Strain Square CT
Knightdale NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 2nd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



EAB
Signature of Certifying Official

671
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: 008838
Test Date: 02/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Bryant Jr., Earl A
Permit Number: 0017-9707
Effective:
09/15/2020-09/15/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG018401
Exp Date: 07/02/2022

Test	g/210L	Time
DIAG	Pass	1:19pm
AIR BLK	.00	1:20pm
ACCY CHK	.07	1:21pm
AIR BLK	.00	1:22pm
SUB TEST	.00	1:22pm
AIR BLK	.00	1:23pm
SUB TEST	.00	1:24pm
AIR BLK	.00	1:25pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY KNIGHTDALE PD 910

Serial Number: 008838 Test Record Number: 2077
Test Date: 02/03/2021 Test Time: 1:26pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:27pm
FLO	Pass	1:27pm
FC	Pass	1:27pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:27pm
SRC	Pass	1:27pm
DET	Pass	1:27pm
BAR	Pass	1:27pm
BT	Pass	1:27pm

Blank Tests

Test	Status	Time
AIR	Pass	1:28pm

Printer Tests

Test	Status	Time
PRNT	Pass	1:28pm

CRC Tests

Test	Status	Time
COMP	Pass	1:28pm
CAL	Pass	1:28pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wake Instrument Location Wake Co Detention Ctr

Instrument Serial No. 008924 3301 Hammond Rd Raleigh NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 28 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Handwritten Signature]

Signature of Certifying Official

662

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008924
Test Date: 02/28/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Barnes, Simon S
Permit Number: 0014-6221
Effective:
09/01/2020-09/01/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG034902
Exp Date: 12/14/2022

Test	g/210L	Time
DIAG	Pass	12:39pm
AIR BLK	.00	12:40pm
ACCY CHK	.08	12:41pm
AIR BLK	.00	12:42pm
SUB TEST	.00	12:42pm
AIR BLK	.00	12:43pm
SUB TEST	.00	12:45pm
AIR BLK	.00	12:45pm

Reported AC: .00 g/210L


Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008924 Test Record Number: 1568
Test Date: 02/28/2021 Test Time: 12:46pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	12:47pm
FLO	Pass	12:47pm
FC	Pass	12:47pm

Temperature Tests

Test	Status	Time
FC1	Pass	12:47pm
SRC	Pass	12:47pm
DET	Pass	12:47pm
BAR	Pass	12:47pm
BT	Pass	12:47pm

Blank Tests

Test	Status	Time
AIR	Pass	12:48pm


Printer Tests

Test	Status	Time
PRNT	Pass	12:48pm

CRC Tests

Test	Status	Time
COMP	Pass	12:48pm
CAL	Pass	12:48pm

Preventive Maintenance
Status: Pass

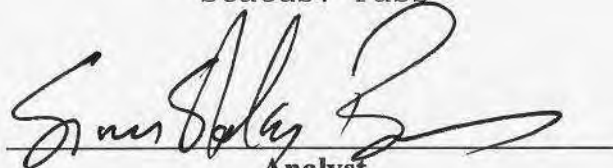
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County WASHINGTON Instrument Location WASHINGTON CO. S.D.

Instrument Serial No. 008829 120 ADAM ST., PLYMOUTH, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3RD day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



John A. Reese
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829
Test Date: 02/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Keesler, Linda A
Permit Number: 0045-5468
Effective:
09/16/2020-09/16/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG081202
Exp Date: 06/30/2022


Test	g/210L	Time
DIAG	Pass	12:54pm
AIR BLK	.00	12:55pm
ACCY CHK	.08	12:55pm
AIR BLK	.00	12:56pm
SUB TEST	.00	12:56pm
AIR BLK	.00	12:57pm
SUB TEST	.00	12:59pm
AIR BLK	.00	1:00pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WASHINGTON COUNTY SHERIFF'S OFFICE 930

Serial Number: 008829 Test Record Number: 1033
Test Date: 02/03/2021 Test Time: 1:01pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:01pm
FLO	Pass	1:01pm
FC	Pass	1:01pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:01pm
SRC	Pass	1:01pm
DET	Pass	1:01pm
BAR	Pass	1:01pm
BT	Pass	1:01pm

Blank Tests

Test	Status	Time
AIR	Pass	1:02pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:02pm

CRC Tests

Test	Status	Time
COMP	Pass	1:02pm
CAL	Pass	1:02pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County WAYNE Instrument Location SEYMOUR JOHNSON A.F.B.
Instrument Serial No. 008786 1010 VERMONT GARRISON RD.
BOLESBORO, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 25th day of FEBRUARY, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linda Kure
Signature of Certifying Official

647
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: 008786
Test Date: 02/25/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Keesler, Linda A
Permit Number: 0045-5468
Effective:
09/16/2020-09/16/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG007601
Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	2:14pm
AIR BLK	.00	2:15pm
ACCY CHK	.08	2:15pm
AIR BLK	.00	2:16pm
SUB TEST	.00	2:17pm
AIR BLK	.00	2:18pm
SUB TEST	.00	2:19pm
AIR BLK	.00	2:20pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY SEYMOUR JOHNSON AFB 950

Serial Number: 008786 Test Record Number: 358
Test Date: 02/25/2021 Test Time: 2:10pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:11pm
FLO	Pass	2:11pm
FC	Pass	2:11pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:11pm
SRC	Pass	2:11pm
DET	Pass	2:11pm
BAR	Pass	2:11pm
BT	Pass	2:11pm

Blank Tests

Test	Status	Time
AIR	Pass	2:12pm


Printer Tests

Test	Status	Time
PRNT	Pass	2:12pm

CRC Tests

Test	Status	Time
COMP	Pass	2:12pm
CAL	Pass	2:12pm

Preventive Maintenance
Status: Pass


Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)

County Wilkes Instrument Location Wilkes Co. Detention
Instrument Serial No. 008843 Wilkesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

649
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008843
Test Date: 02/16/2021

Citation Number: M0000000-0
Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J

Permit Number: 0018-4401

Effective:

10/01/2020-10/01/2022

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG933901

Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	2:51pm
AIR BLK	.00	2:52pm
ACCY CHK	.08	2:53pm
AIR BLK	.00	2:54pm
SUB TEST	.00	2:55pm
AIR BLK	.00	2:56pm
SUB TEST	.00	2:58pm
AIR BLK	.00	2:59pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures
Forensic Tests for Alcohol Branch
Department of Health and Human Services
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008843 Test Record Number: 2541
Test Date: 02/16/2021 Test Time: 2:59pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:00pm
FLO	Pass	3:00pm
FC	Pass	3:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:00pm
SRC	Pass	3:00pm
DET	Pass	3:00pm
BAR	Pass	3:00pm
BT	Pass	3:00pm

Blank Tests

Test	Status	Time
AIR	Pass	3:01pm

Printer Tests

Test	Status	Time
PRNT	Pass	3:01pm

CRC Tests

Test	Status	Time
COMP	Pass	3:01pm
CAL	Pass	3:01pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wilkes Instrument Location Wilkes Co. Detention
Instrument Serial No. 008865 Wilkesboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass" and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of February, 2021 the foregoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

[Signature]
Technician Name

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008865
Test Date: 02/16/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE

Analyst's Name: Burnette, Anthony J
Permit Number: 0018-4401
Effective:
10/01/2020-10/01/2022

Officer's Name: NONE,
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG933901
Exp Date: 12/05/2021

Test	g/210L	Time
DIAG	Pass	2:52pm
AIR BLK	.00	2:53pm
ACCY CHK	.08	2:54pm
AIR BLK	.00	2:55pm
SUB TEST	.00	2:55pm
AIR BLK	.00	2:56pm
SUB TEST	.00	2:58pm
AIR BLK	.00	2:59pm

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR


Analyst

Intox EC/IR-II: Preventive Maintenance

WILKES COUNTY WILKES CO DETENTION 960

Serial Number: 008865 Test Record Number: 812
Test Date: 02/16/2021 Test Time: 3:00pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	3:00pm
FLO	Pass	3:00pm
FC	Pass	3:00pm

Temperature Tests

Test	Status	Time
FC1	Pass	3:00pm
SRC	Pass	3:00pm
DET	Pass	3:00pm
BAR	Pass	3:00pm
BT	Pass	3:00pm

Blank Tests

Test	Status	Time
AIR	Pass	3:01pm


Printer Tests

Test	Status	Time
PRNT	Pass	3:01pm

CRC Tests

Test	Status	Time
COMP	Pass	3:01pm
CAL	Pass	3:01pm

Preventive Maintenance
Status: Pass

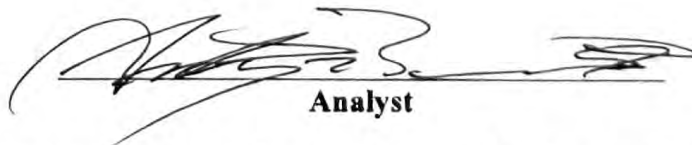

Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)


County Wilson Instrument Location Wilson Co. Detention Center

Instrument Serial No. DD 8627 100 E Green St, Wilson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 31st day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]
Signature of Certifying Official

1643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627
Test Date: 02/03/2021

Citation Number: M0000000-0
Subject's Name:
PREVENTIVE, MAINTENANCE
Subject's Date of Birth: 11/11/1911
Subject's Sex: Male
Driver's License State: XX
Driver's License Number: NONE


Analyst's Name: Guard, Kelly G
Permit Number: 0037-7722
Effective:
09/28/2020-09/28/2022

Officer's Name: NONE, NONE
Type of Agency: FTA
Agency: DHHS
Test Type: Breath Test

Lot Number: AG035001
Exp Date: 12/15/2022

Test	g/210L	Time
DIAG	Pass	2:03pm
AIR BLK	.00	2:03pm
ACCY CHK	.08	2:04pm
AIR BLK	.00	2:05pm
SUB TEST	.00	2:07pm
AIR BLK	.00	2:08pm
SUB TEST	.00	2:10pm
AIR BLK	.00	2:11pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008627 Test Record Number: 2697
Test Date: 02/03/2021 Test Time: 2:12pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	2:12pm
FLO	Pass	2:12pm
FC	Pass	2:12pm

Temperature Tests

Test	Status	Time
FC1	Pass	2:13pm
SRC	Pass	2:13pm
DET	Pass	2:13pm
BAR	Pass	2:13pm
BT	Pass	2:13pm

Blank Tests

Test	Status	Time
AIR	Pass	2:13pm

Printer Tests

Test	Status	Time
PRNT	Pass	2:13pm

CRC Tests

Test	Status	Time
COMP	Pass	2:13pm
CAL	Pass	2:13pm

Preventive Maintenance
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD
INTOXIMETERS, MODEL INTOX EC/IR II and
MODEL INTOX EC/IR II (Enhanced with serial number 10,000 or higher)**

County Wilson Instrument Location Wilson Co. Detention Center
Instrument Serial No. 008652 110 E. Green St, Wilson, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II and Model Intox EC/IR II (Enhanced with serial number 10,000 or higher) to be followed at least once every four months are:

- (1) Verify the ethanol gas canister displays at least 51 pounds per square inch (psi) of pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
- (2) Verify instrument displays time and date;
- (3) Initiate breath test sequence;
- (4) Enter information as prompted;
- (5) Verify instrument accuracy;
- (6) When "PLEASE BLOW" appears, collect breath sample;
- (7) When "PLEASE BLOW" appears, collect breath sample;
- (8) Print test record;
- (9) Run diagnostic program and confirm preventive maintenance status of "Pass"; and
- (10) Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 3rd day of February, 2021 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Key
Signature of Certifying Official

643
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652
Test Date: 02/03/2021

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: Guard, Kelly G

Permit Number: 0037-7722

Effective:

09/28/2020-09/28/2022

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG007601

Exp Date: 03/16/2022

Test	g/210L	Time
DIAG	Pass	1:44pm
AIR BLK	.00	1:45pm
ACCY CHK	.08	1:46pm
AIR BLK	.00	1:47pm
SUB TEST	.00	1:48pm
AIR BLK	.00	1:49pm
SUB TEST	.00	1:50pm
AIR BLK	.00	1:51pm

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

Intox EC/IR-II: Preventive Maintenance

WILSON COUNTY DETENTION CENTER 970

Serial Number: 008652 Test Record Number: 3505
Test Date: 02/03/2021 Test Time: 1:53pm EST

System Check: *Passed*

Baseline Tests

Test	Status	Time
IR	Pass	1:53pm
FLO	Pass	1:53pm
FC	Pass	1:53pm

Temperature Tests

Test	Status	Time
FC1	Pass	1:53pm
SRC	Pass	1:53pm
DET	Pass	1:53pm
BAR	Pass	1:53pm
BT	Pass	1:53pm

Blank Tests

Test	Status	Time
AIR	Pass	1:54pm


Printer Tests

Test	Status	Time
PRNT	Pass	1:54pm

CRC Tests

Test	Status	Time
COMP	Pass	1:54pm
CAL	Pass	1:54pm

Preventive Maintenance
Status: Pass



Analyst